

Los Alamos

Radiation Monitoring

Notebook



James T. (Tom) Voss, NRRPT, CHP
Fellow of the Health Physics Society
2015 Update

| | |
|--|-----|
| Abbreviations | 114 |
| Activity vs Exposure Rate | 30 |
| Activity vs Particle Size | 40 |
| Acute Radiation Effects | 5 |
| Airborne Radioactivity | 65 |
| Characteristic X-Rays of the Elements | 101 |
| Comparative Risk of Radiation Exposure | 142 |
| Composition of Air | 112 |
| Composition of the Human Body | 43 |
| Constants | 120 |
| Contamination Limits | 63 |
| Conversion of Units | 115 |
| Dosimetry | 44 |
| Elevation of Major Airports and Facilities | 109 |
| Elevation vs Air Pressure | 108 |
| Electromagnetic Spectrum | 122 |
| Emergency Response | 1 |
| Equations and Formulas | 59 |
| Inhalation DAC Factors & ALIs for Ingestion & Inhalation | 71 |
| Instrument Selection | 64 |
| Positron Emitters | 54 |
| Public Radiation Doses | 140 |
| Radiation Biology | 43 |
| Radiation Interactions | 50 |
| Radiation Shielding | 51 |
| Radioactive Decay Modes and Decay Chains | 9 |
| Radon | 141 |
| Rules of Thumb | 123 |
| SI & US Units | 113 |
| Statistics | 105 |
| Surface and Volume Calculations | 121 |
| Table of the Elements | 7 |
| Units and Terminology | 139 |
| Websites of Interest | 144 |

Author's notes

Over my career in health physics starting with a US Army CBR unit at Dugway Proving Ground in 1965 I have needed to quickly find that elusive data point that I just couldn't remember, even though I knew the information was in one of my several hundred reference books.

So, here it is today, the product of my work to assemble useful field information from a wide range of sources.

I must give credit to those individuals who put their efforts into creating the original data. Without their work, this document could not have been assembled.

My family has given me their unlimited support in my development of this reference book and in my projects all through my career. Sandy my wife of 40 years and our two daughters Susan and Sarah and their excellent husbands, Bill Gilson and Rolfe Bergstrom, our son-in-laws, continue to provide me with a steady foundation that allows me to try out new concepts.

James T. (Tom) Voss, NRRPT, CHP
Fellow of the Health Physics Society
Northern New Mexico, 2015

Send your corrections, additions, deletions, and comments to:

JTVOSS@NEWMEXICO.COM

WWW.VOSS-ASSOCIATES.COM

RADIOLOGICAL EMERGENCY RESPONSE

Write in Your Emergency Phone Numbers

Supervisor:

Team Office:

Group Office:

Division Office:

Emergency Response Team:

Fire Department:

Hospital:

Guidelines for Control of Emergency Exposures

Use a dose limit of: (EPA-400)

- | | |
|--------------------|--|
| 5 rem (50 mSv) | for all emergency procedures |
| 10 rem (100 mSv) | only for protecting major property |
| 25 rem (250 mSv) | for lifesaving or protection of large populations |
| > 25 rem (250 mSv) | for lifesaving or protection of large populations only by volunteers and where the risks have been evaluated |

EMERGENCY RESPONSE

SWIMS for Radiological and Other Emergencies

Only under extreme radiological conditions such as external radiation greater than 100 rem / hr (1 Sv/h) or airborne radioactivity concentrations greater than 100,000 DAC would the radiological emergency take precedence over serious personnel injuries.

Hazardous conditions such as atmospheres that are IDLH (Immediately Dangerous to Life or Health) would require you to implement controls to protect the emergency responders.

Therefore, you would not attempt to move a seriously injured person before medical personnel arrived unless the radiological or other hazardous condition presented a greater danger to that person and yourself.

Stay or **S**ecure operations in the area. If applicable, secure the operation causing the emergency.

Warn others in the area as you are evacuating. Do not search for potentially missing personnel at this stage of the emergency.

Isolate the source of the radiation or radioactivity or other contaminant or hazard only if you understand the operation and are qualified to isolate the source.

Minimize individual exposure and contamination. Control the entry points to the area if possible.

Secure unfiltered ventilation. Evaluate the radiological or other hazardous condition and advise facility personnel on ventilation control.

HAZARD CONTROL PRIORITIES DURING MEDICAL EMERGENCIES

Immediate treatment by trained medical personnel should be sought for any serious injuries such as those involving profuse bleeding or broken bones. The order of priority should be to protect lives, protect property, and then to control the spread of contamination.

Identifying a Major Injury

Consider the following points in determining if the injury should be handled as a major injury.

- Any head injury (from base of neck to top of head)
- Any loss of consciousness
- Any disorientation
- Any convulsion
- Any loss of sensation
- Any loss of motor function
- Limbs at abnormal angles
- Amputations
- Any burn of the face, hands, feet, or genitals (chemical, thermal, or radiation)
- Any burn larger than the palm of your hand
- Any inhalation of any abnormal substance
- Profuse bleeding
- Abnormal breathing patterns

Major Injuries Occurring in Hazardous Areas

Protect yourself - consider the magnitude of any radiation field, airborne contamination, or other hazard.

Stay with the injured person unless doing so puts you at immediate risk to life or health.

Don't move the injured person unless there is a danger from some environmental emergency such as fire, explosion, hazardous material spill, or radiation field.

If you must move the injured person, drag them by either the hands or the feet to a safe area.

Apply First Aid Only if you are trained to do so.

Secure help - yell or phone, but don't leave the injured person unless necessary.

Send someone to meet the ambulance to guide the medical personnel to the injured person.

Prepare the area for access by the medical team.

Begin a gross hazard evaluation of the immediate area near the injured person, beginning with the injured person.

Be sure to survey any object that caused the injury.

Provide information to medical personnel about the injured person (what happened, how, when, location of phone and exits, indicate which areas on the injured person are contaminated and include contamination values).

ACUTE RADIATION EFFECTS

0 – 25 REM (0 - 0.25 Sv)

minimal decrease in white blood cell count for ~ 2 weeks
increase in risk of dying from cancer from US average risk of ~ 14 persons per 100 population to ~ 17 persons per 100 population (3 additional persons per 100 population will experience the onset of terminal cancer ~25 years after the acute exposure)

> 25 REM - < 100 REM (0.25 - 1 Sv)

small decrease in white blood cell count for > 2 weeks
increase in risk of dying from cancer to ~ 26 in 100

> 100 REM - < 200 REM (1 - 2 Sv)

moderate decrease in white blood cell count
25% of those exposed will experience nausea within a few hours
less than 5% of those exposed require hospitalization
increase in risk of dying from cancer to ~ 38 in 100

> 200 REM - < 600 REM (2 - 6 Sv)

major decrease in white blood cell count
~ 100% of those exposed will experience nausea within a few hours
appearance of bruises on skin (purpura)
pneumonia symptoms
hair loss
90% of those exposed require hospitalization
decrease in thinking ability for ~ 2 weeks
increase in risk of dying from cancer to ~ 74 in 100

600 REM - < 800 REM (6 - 8 Sv)

all of the above symptoms will be present

100% of those exposed require hospitalization

~ 100% of those exposed will die within a few weeks without medical treatment

increase in risk of dying from cancer to ~ 98 in 100

800 REM - < 2000 REM (8 - 20 Sv)

all of the above symptoms will be present

diarrhea, fever, electrolytes imbalance, GI tract and respiratory system failure

100% of those exposed will be incapacitated within hours

very few of those exposed will survive

> 2000 REM (> 20 Sv)

100% mortality within a few days

TERMS

Lymphocyte - white blood cells

Leukopenia - abnormally low white blood cell count

Purpura - purple discoloration of skin caused by blood bleeding into the skin tissue

Pneumonia - inflammation of lung tissue, accompanied by fever, chills, cough, and difficulty in breathing

Hematopoietic – decrease in the formation of blood cells

Ataxia - inability to coordinate voluntary muscular movements

BEIR V 1990 800 excess deaths per 100,000 persons at 10 rem
(4,000 Hiroshima survivors in excess of 50 rem dose had an extra 300 incidences of cancer)

(~ 7500 excess deaths per 100,000 at 50 rem)

(~ 1500 excess deaths per 100,000 at 10 rem)

TABLE OF THE ELEMENTS

| Z | | | Density | Z | | | Density (g/cc) |
|----------|-------------|----|----------------|----------|-------------|----|-----------------------|
| 89 | Actinium | Ac | 10.07 | 64 | Gadolinium | Gd | 7.90 |
| 13 | Aluminum | Al | 2.6989 | 31 | Gallium | Ga | 5.9 |
| 95 | Americium | Am | 13.67 | 32 | Germanium | Ge | 5.32 |
| 51 | Antimony | Sb | 6.618 | 79 | Gold | Au | 19.32 |
| 18 | Argon | Ar | 0.0018 | 72 | Hafnium | Hf | 13.31 |
| 33 | Arsenic | As | 5.727 | 105 | Hahnium | Ha | ~ 18 |
| 85 | Astatine | At | ~ 15 | 2 | Helium | He | 1.8E-4 |
| 56 | Barium | Ba | 3.51 | 67 | Holmium | Ho | 8.795 |
| 97 | Berkelium | Bk | 14 | 1 | Hydrogen | H | 9E-5 |
| 4 | Beryllium | Be | 1.848 | 49 | Indium | In | 7.31 |
| 83 | Bismuth | Bi | 9.747 | 53 | Iodine | I | 4.93 |
| 5 | Boron | B | 2.37 | 77 | Iridium | Ir | 22.42 |
| 35 | Bromine | Br | 3.12 | 26 | Iron | Fe | 7.87 |
| 48 | Cadmium | Cd | 8.65 | 36 | Krypton | Kr | 0.0037 |
| 20 | Calcium | Ca | 1.55 | 57 | Lanthanum | La | 6.15 |
| 98 | Californium | Cf | ~ 18 | 103 | Lawrencium | Lr | ~ 18 |
| 6 | Carbon | C | 2.05 | 82 | Lead | Pb | 11.35 |
| 58 | Cerium | Ce | 6.67 | 3 | Lithium | Li | 0.534 |
| 55 | Cesium | Cs | 1.873 | 71 | Lutetium | Lu | 9.84 |
| 17 | Chlorine | Cl | 0.0031 | 12 | Magnesium | Mg | 1.738 |
| 24 | Chromium | Cr | 7.19 | 25 | Manganese | Mn | 7.43 |
| 27 | Cobalt | Co | 8.9 | 101 | Mendelevium | Mv | ~ 18 |
| 29 | Copper | Cu | 8.96 | 80 | Mercury | Hg | 13.546 |
| 96 | Curium | Cm | 13.51 | 42 | Molybdenum | Mo | 10.22 |
| 66 | Dysprosium | Dy | 8.54 | 60 | Neodymium | Nd | 7.008 |
| 99 | Einsteinium | Es | ~ 18 | 10 | Neon | Ne | 0.0009 |
| 68 | Erbium | Er | 9.066 | 93 | Neptunium | Np | 20.25 |
| 63 | Europium | Eu | 5.244 | 28 | Nickel | Ni | 8.9 |
| 100 | Fermium | Fm | ~ 18 | 41 | Niobium | Nb | 8.57 |
| 9 | Fluorine | F | 0.0017 | 7 | Nitrogen | N | 0.00125 |
| 87 | Francium | Fr | ~ 15 | 102 | Nobelium | No | ~ 18 |

| Z | | | Density | Z | | | Density (g/cc) |
|-----|---------------|----|---------|----|------------|----|----------------|
| 76 | Osmium | Os | 22.57 | 14 | Silicon | Si | 2.3 |
| 38 | Oxygen | O | 0.00143 | 47 | Silver | Ag | 10.5 |
| 46 | Palladium | Pd | 12.02 | 11 | Sodium | Na | 0.97 |
| 15 | Phosphorus | P | 2.2 | 38 | Strontium | Sr | 2.54 |
| 78 | Platinum | Pt | 21.45 | 16 | Sulfur | S | 2.0 |
| 94 | Plutonium | Pu | 19.84 | 73 | Tantalum | Ta | 16.6 |
| 84 | Polonium | Po | 9.32 | 43 | Technetium | Tc | 11.5 |
| 19 | Potassium | K | 0.862 | 52 | Tellurium | Te | 6.24 |
| 59 | Praseodymium | Pr | 6.773 | 65 | Terbium | Tb | 8.27 |
| 61 | Promethium | Pm | 7.264 | 81 | Thallium | Tl | 11.85 |
| 91 | Protactinium | Pa | 15.37 | 90 | Thorium | Th | 11.70 |
| 88 | Radium | Ra | 5.5 | 69 | Thulium | Tm | 9.321 |
| 86 | Radon | Rn | 0.0097 | 50 | Tin | Sn | 6.5 |
| 75 | Rhenium | Re | 21.02 | 22 | Titanium | Ti | 4.54 |
| 45 | Rhodium | Rh | 12.41 | 74 | Tungsten | W | 19.3 |
| 37 | Rubidium | Rb | 1.532 | 92 | Uranium | U | 16.95 |
| 44 | Ruthenium | Ru | 12.41 | 23 | Vanadium | V | 6.11 |
| 104 | Rutherfordium | Rf | ~18 | 54 | Xenon | Xe | 0.0059 |
| 62 | Samarium | Sm | 7.54 | 70 | Ytterbium | Yb | 6.98 |
| 21 | Scandium | Sc | 2.989 | 39 | Yttrium | Y | 4.47 |
| 106 | Seaborgium | Sg | ~18 | 30 | Zinc | Zn | 7.13 |
| 34 | Selenium | Se | 4.5 | 40 | Zirconium | Zr | 6.06 |

RADIOACTIVITY

| | | |
|-------------|----------------------|---|
| zX^A | Z = | atomic # (number of protons) |
| | X = | element |
| | A = | mass # (number of protons and neutrons) |
| Decay Modes | Alpha | $zX^A \rightarrow z-2X^{A-4} + \alpha$ |
| | Beta Minus | $zX^A \rightarrow z+1X^A + \beta^-$ |
| | Beta Plus (Positron) | $zX^A \rightarrow z-1X^A + \beta^+$ |
| | Electron Capture | $zX^A \rightarrow z-1X^A$ |

Relative Locations of Products of Nuclear Processes

| | | | | |
|---------------|-------------------|---|-----------------------------|---|
| | | He^3 in | α in | |
| β^- out | p in | d in | t in | |
| η out | Original Nucleus | η in | | |
| t out | d out | p out | β^+ out ϵ | |
| α out | He^3 out | η neutron t triton (H^3) β^+ positron | p proton α alpha | d deuteron β^- beta ϵ electron capture |

Use this chart along with the Table of the Elements to determine the progeny (and ancestor) of an isotope. For example; we know Pu^{238} is an alpha emitter. The alpha decay mode tells us the mass # decreases by 4 (238 goes to 234) and the Z # decreases by two (94 goes to 92). The element with a Z # of 92 is Uranium. Pu^{238} decays to U^{234} . As another example; we know Cl^{36} is a beta emitter. The beta decay mode tells us the mass # stays the same and the Z # increases by one (17 goes to 18). The element with a Z # of 18 is Argon. Cl^{36} decays to Ar^{36}

Radioactive Decay Calculation

$$A_t = A_0 e^{-\lambda t}$$

$$A_0 = A_t / e^{-\lambda t}$$

$$t = \ln(A_t/A_0) / -\lambda \quad \text{half-life} = -t \times 0.693 / \ln(A_t/A_0)$$

Where; A_t is the activity at the end of time 't'

A_0 is the activity at the beginning

λ is 0.693 divided by the half-life

t is the decay time

Example: What is the % activity of Co-60 remaining 12 years after it was produced ?

Co-60 half-life is 5.271 years

$$A_t = A_0 e^{-\lambda t}$$

$$A_t = 100 e^{-0.693/5.271 \times 12} = 100 e^{-1.578} = 100 \times 0.206 = 20.6\%$$

Calculating the Activity of Progeny

$$A_{dt} = A_{p(0)} \times \lambda_d / (\lambda_d - \lambda_p) \times (e^{-\lambda_p t} - e^{-\lambda_d t})$$

$A_{d(t)}$ is the activity of the progeny at the end of time 't'

$A_{p(0)}$ is the activity of the parent at the beginning

Example: What is the activity of Tc-99m 14 hours after its parent Mo-99 was produced ?

Mo-99 half-life is 66.02 minutes, initial activity is 100 uCi

Tc-99m half-life is 6.0058 hours, initial activity is 0 uCi

$$A_{dt} = 100 \text{ uCi} \times 0.693/6.0058 / (0.693/6.0058 - 0.693/66.02) \times (e^{-0.693/66.02 \times 14} - e^{-0.693/6.0058 \times 14})$$

$$A_{dt} = 100 \text{ uCi} \times 1.149 \times (0.8633 - 0.1989) = 76.3 \text{ uCi Tc-99m}$$

Note: IF the progeny has activity at time '0', the decrease in activity of the progeny must be accounted for with an additional calculation.

COMMONLY ENCOUNTERED RADIONUCLIDES

Only the most abundant energies are listed. ‘S’ is “Stable”

| | Progeny | | kev and % abundance |
|-----------------------------|-----------------------|---------------------|--|
| H ³ 12.32y | He ³ S | β ⁻ | 18.6 (100) |
| Be ⁷ 53.44d | Li ⁷ S | EC γ | |
| C ¹⁴ 5730y | N ¹⁴ S | β ⁻ | 157 (100) |
| O ¹⁵ 122.24s | N ¹⁵ S | β ⁺ γ | 1732 (99.9) 511 (200) |
| N ¹⁶ 7.13s | O ¹⁶ S | β ⁻ γ | 3302 (4.9), 4288 (68), 10418 (26) 6129 (69), 7115 (5) |
| F ¹⁸ 109.74m | O ¹⁸ S | β ⁺ γ | 634 (96.73) 511 194) |
| Na ²² 2.602y | Ne ²² S | β ⁺ γ | 546 (89.84) 1275 (99.94) |
| | | Ne x-rays | 1 (0.12) |
| Na ²⁴ 15.00h | Mg ²⁴ S | β ⁻ γ | 1390 (99.935) 1369 (99.9991), 2754 (99.862) |
| Al ²⁶ 7.17E5y | Mg ²⁶ S | β ⁺ γ | 1174 (81.81) 130 (2.5), 1809 (99.96), 2938 (0.24) |
| | | Mg x-rays | 1 (0.44) |

| | | | |
|-----------------------------|--|--|--|
| P ³² 14.29d | S ³² S | β^- | 1710 (100) |
| Cl ³⁶ 3.01E5y | Ar ³⁶ S | β^- | 710 (99.0) |
| K ⁴⁰ 1.27E9y | Ca ⁴⁰ S Ar ⁴⁰ S | β^- EC γ Ar x-rays | 1312 (89.33) 1461 (10.67) 3 (0.94) |
| Ar ⁴¹ 1.827h | K ⁴¹ S | β^- γ | 1198 (99.17), 2492 (0.78) 1294 (99.16) |
| K ⁴² 12.36h | Ca ⁴² S | β^- γ | 1684(0.32), 1996(17.5), 3521(82.1) 313(0.3), 1525 (18) |
| K ⁴³ 22.6h | Ca ⁴³ S | β^- γ | 422 (2.24), 827 (92.2), 1224 (3.6) 373 (87.3), 397 (11.43), 593 (11.0), 617 (80.5) |
| Sc ⁴⁶ 83.83d | Ti ⁴⁶ S | β^- γ | 357 (99.996) 889 (99.983), 1121 (99.987) |
| Sc ⁴⁷ 3.351d | Ti ⁴⁷ S | β^- γ | 441 (68), 601 (32) 159 (68) |
| Sc ⁴⁸ 43.7h | Ti ⁴⁸ S | β^- γ | 482 (10.01), 657 (89.99) 984 (100), 1037 (97.5), 1312 (100) |

| | | | |
|-----------|-----------|------------|---|
| V^{48} | Ti^{48} | β^+ | 697 (50.1) |
| 16.238d | S | γ | 944 (7.76), 984 (100), 1312 (97.5) |
| | | Ti x-rays | 0.45 (0.15), 5 (9.74) |
| Cr^{51} | V^{51} | EC | |
| 27.704d | S | γ | 320 (9.83) |
| | | V x-rays | 1 (0.33), 5 (22.31) |
| Mn^{52} | Cr^{52} | β^+ | 575 (29.4) |
| 5.591d | S | γ | 511(67), 744(82), 935(84), 1434(100) |
| | | Cr x-rays | 1 (0.26), 5 (15.5), 6 (2.94) |
| Mn^{54} | Cr^{54} | EC | |
| 312.5d | S | γ | 835 (99.975) |
| | | Cr x-rays | 1 (0.37), 5 (22.13), 6 (2.94) |
| Fe^{55} | Mn^{55} | EC | |
| 2.7y | S | Mn x-rays | 1 (0.42), 6 (24.5), 6 (3.29) |
| Mn^{56} | Fe^{56} | β^- | 736 (14.6), 1038 (27.8), 2849 (56.2) |
| 2.5789h | S | γ | 847 (98.9), 1811 (27.2), 2113 (14.3) |
| Co^{56} | Fe^{56} | β^+ | 423 (1.05), 1461 (18.7) |
| 78.76d | S | γ | 847 (99.958), 10381 (14.03), 1238 (67), 1771 (15.5), 2598 (16.9) |
| | | Fe x-rays | 1 (0.34), 6 (21.83), 7 (2.92) |
| Ni^{57} | Co^{57} | β^+ | 463 (0.87), 716 (5.7), 843 (33.1) |
| 35.60h | S | γ | 127 (12.9), 1378 (77.9), 1919 (14.7) |
| | | Co x-rays | 1 (0.29), 7 (18.1), 8 (2.46) |

| | | | |
|-----------------------------|-----------------------|--|--|
| Co^{57} 270.9d | Fe^{57} S | EC γ Fe x-rays | 14 (9.54), 122 (85.51), 136 (10.6) 1 (0.8), 6 (49.4), 7 (6.62) |
| Co^{58} 70.8d | Fe^{58} S | β^+ γ Fe x-rays | 475 (14.93) 811 (99.4), 864 (0.74), 1675 (0.54) 0.7 (0.36), 6 (23.18), 7 (3.1) |
| Ni^{59} 7.5E4y | Co^{59} S | EC Co x-rays | 1 (0.47), 7 (29.8) |
| Fe^{59} 44.53d | Co^{59} S | β^- γ | 131 (1.37), 273 (45.2), 466 (53.1) 192 (3.11), 1099 (56.5). 1292 (43.2) |
| Co^{60} 5.271y | Ni^{60} S | β^- γ | 318 (100) 1173 (100), 1332 (100) |
| Cu^{62} 9.673m | Ni^{62} S | β^- γ Ni x-rays | 1754 (0.132), 2927 (97.59) 876 (0.148), 1173 (0.336) 7 (0.7) |
| Ni^{63} 98.7y | Cu^{63} S | β^- | 66.98 (100) |
| Zn^{65} 243.66d | Cu^{65} S | EC β^+ γ Cu x-rays | 330 (1.415) 1116 (50.75) 1 (0.57), 8 (34.1), 9 (4.61) |
| Ni^{65} 2.520h | Cu^{65} S | β^- γ | 2130 (100) 368 (4.5), 1115 (16), 1481 (25) |

| | | | |
|------------------|------------------|-----------|--------------------------------------|
| Ge^{68} | Ga^{68} | EC | |
| 270.9d | | Ga x-rays | 1 (0.67), 9 (38.7), 10 (5.46) |
| Ga^{68} | Zn^{68} | β^+ | 822 (0.012), 1899 (0.8794) |
| 67.7m | S | γ | 1077 (0.032), 1883 (0.0014) |
| | | Zn x-rays | 9 (0.049), 10 (0.00579) |
| As^{74} | Se^{74} | β^- | 1353 (34.0) |
| 17.77d | S | γ | 634 (15.4) |
| | Ge^{74} | EC | |
| | S | β^+ | 1540 (66.0) |
| | | γ | 596 (59.9), 608 (0.55), 1204 (0.287) |
| | | Ge x-rays | 1 (0.26), 10 (15), 11 (2.22) |
| Se^{75} | As^{75} | EC | |
| 119.78d | S | γ | 136 (59.2), 265 (59.8), 280 (25.2) |
| | | As x-rays | 1 (0.9), 11 (47.5), 12 (7.3) |
| Kr^{85} | Rb^{85} | β^- | 173 (0.437), 687 (99.563) |
| 10.72y | S | γ | 514 (0.434) |
| Rb^{88} | Sr^{88} | β^- | 2581 (13.3), 3479 (4.1), 5315 (7.8) |
| 17.772m | S | γ | 898 (14), 1836 (21.4), 2678 (1.98) |
| Rb^{89} | Sr^{89} | β^- | 1275 (33), 2223 (34), 4503 (25) |
| 15.15m | | γ | 1031 (58), 1248 (42), 2196 (13.3) |
| Sr^{89} | Y^{89} | β^- | 1491 (99.985) |
| 50.53m | S | γ | av. 909 (0.02) |
| Sr^{90} | Y^{90} | β^- | 546 (100) |
| 28.9y | | | |
| Y^{90} | Zr^{90} | β^- | 519 (0.0115), 2284 (99.9885) |
| 64.00h | S | | |

| | | | |
|--|---------------------------------|-----------------------|---|
| Nb^{94} 20.3E4y | Mo^{94} S | β^- γ | 471 (100) 703 (100), 871 (100) |
| Zr^{95} 63.98d | Nb^{95} | β^- | 366 (55.4), 399 (43.7), 887 (0.78) |
| Nb^{95} 34.991d | Mo^{95} S | γ β^- | 724 (43.7), 757 (55.3) 160 (99.97) 766 (100) |
| Mo^{99} decays 88.6% of the time to Tc^{99m} and 11.4% to Tc^{99} . | | | |
| 66.0h | | β^- | 436 (17.3), 848 (1.36), 1214 (82.7) |
| | | γ | 181 (6.2), 740 (12.8), 778 (4.5) |
| | | Tc x-rays | 2 (0.2), 18 (2.63), 21 (0.52) |
| Tc^{99m} 6.0058h | Tc^{99} | γ | 141 (89.07) |
| Tc^{99} 2.13E5y | Ru^{99} S | β^- | Tc x-rays 294 (99.998) |
| Ru^{106} 371.8d | Rh^{106} | β^- | 39 (100) |
| Rh^{106} 29.9s | Pd^{106} S | β^- γ | 1979(1.77), 2410(10.6), 3541(86.8) 616 (0.75), 622 (9.93), 873 (0.439), 1050 (1.56), 1128 (0.404), 1562 (0.163) |
| Cd^{109} 1.264y | Ag^{109} S | EC γ | 88.03 (100) Ag x-rays 11.28 (12), 12.34 (13) |
| I^{125} 60.1d | Te^{125} S | EC γ | 35 (6.49) Te x-rays 4 (15), 27 (112.2), 31 (25.4) |

| | | | |
|-------------------------------|-----------------------------|-----------|---|
| I ¹²⁶ 12.928d | Xe ¹²⁶ S | β^- | 1258 (47.3) |
| | | γ | 389 (32.1), 491 (2.43), 754 (3.7) |
| | | Xe x-rays | 29 (0.115), 30 (0.213) |
| | Te ¹²⁶ | β^+ | 1132 (52.7) |
| | S | Te x-rays | 4 (4.8), 27 (36.4), 31 (8.2) |
| I ¹²⁹ 1.57E7y | Xe ¹²⁹ S | β^- | 194 (100) |
| | | γ | 40 (7.52) |
| | | Xe x-rays | 4 (12), 29 (29.71), 30 (55), 34 (19.5) |
| I ¹³¹ 8.025d | Xe ¹³¹ S | β^- | 248 (2.1), 334 (7.4), 606 (89.3) |
| | | γ | 80 (2.5), 284 (6.05), 364 (81.2), 637 (7.26), 723 (1.8) |
| | | Xe x-rays | 4 (0.6), 29 (1.3), 30 (2.5), 34 (0.5) |
| I ¹³³ 20.8h | Xe ¹³³ 5.248d | β^- | 371 (1.24), 460 (3.75), 521 (3.12) |
| | | γ | 882(4.16), 1013(1.81), 1227(83.42) 1524 (1.07) |
| | | Xe x-rays | 511 (1.81), 530 (86.3), 707 (1.49), 856(1.23), 875(4.47), 1236(1.49), 1298(2.33) |
| | Cs ¹³³ | β^- | 29 (0.151), 30 (0.281) |
| | S | γ | 267 (0.69), 346 (99.3) |
| | | γ | 530 (86.3), 707 (1.49), 856 (1.23), 875 (4.47), 1236 (1.49), 1298 (2.33) |
| | | Cs x-rays | 81 (37) |
| Ba ¹³³ 10.518yy | Cs ¹³³ S | EC | |
| | | γ | 53 (2.14), 80 (35.55), 276 (6.9), 303 (17.8), 356 (60), 384 (8.7) |
| | | Cs x-rays | 4 (17), 31 (97.6), 35 (22.8) |

| | | | |
|------------------------------|------------------------------|---|---|
| I ¹³⁴ 52.6m | Xe ¹³⁴ S | β^- γ | 1280(32.5), 1560(16.3), 1800(11.2), 2420 (11.5) 847 (95.41), 884 (65.3), 1073 (15.3) Xe x-rays 4(0.17), 29(0.43), 30(0.8), 34(0.3) |
| I ¹³⁵ 6.583h | Xe ¹³⁵ 9.139h | β^- γ | 300 (1.08), 340 (0.91), 350 (1.39), 460 (4.73), 480 (7.33), 620 (1.57), 670 (1.10), 740 (7.9), 920 (8.7), 1030 (21.8), 1150 (7.9), 1250 (7.4), 1450 (23.6), 1580 (1.2), 2180 (1.9) 1132 (22.5), 1260 (28.6), 1678 (9.5) Xe x-rays 30 (0.127) |
| | Cs ¹³⁵ 2.31E6y | β^- γ | 551 (3.13), 751 (0.59), 909 (96.1) 158 (0.29), 249 (89.9), 358 (0.22), 408 (0.36), 608 (2.89) Cs x-rays 4 (0.66), 31 (4.13), 35 (0.96) |
| | Ba ¹³⁵ | β^- γ | 269 (100) 268 (16.0) Ba x-rays 4 (8.6), 32 (43.6), 36 (10.3) |
| Cs ¹³⁷ 30.187y | Ba ^{137m} 2.552m | β^- γ | 512 (94.6), 1173 (5.4) 662 (89.98) S Ba x-rays 4 (1), 32 (5.89), 36 (1.39) |
| Ba ¹⁴⁰ 12.75d | La ¹⁴⁰ 1.68d | β^- γ | 454 (26), 991 (37.4), 1005 (22) 30 (14), 163 (6.7), 537 (25) La x-rays 5 (15), 33 (1.51), 38 (0.36) |
| | Ce ¹⁴⁰ | β^- γ | 1239 (11.11), 1348 (44.5), 1677 (20.7) 329 (20.5), 487 (45.5), 816 (23.5) |
| | Ce x-rays | 5 (0.25), 34 (0.47), 35 (0.9), 39 (0.9) | |

| | | | |
|-----------------------------|--|--|---|
| Gd ¹⁴⁸ 74.52y | Sm ¹⁴⁴ S | α | 3180 (100) |
| Ir ¹⁹² 73.83d | Pt ¹⁹² S | β⁻ γ | 256 (5.65), 536 (41.4), 672 (48.3) 296(29.02), 308(29.68), 317(82.85), 468 (48.1), 589 (4.57), 604 (8.20), 612 (5.34) Pt x-rays 9 (4.1), 65 (2.6), 67 (4.5), 76 (1.97) |
| | Os ¹⁹² S | EC (4.69) Os x-rays 9(1.46), 61(1.1), 63(1.96), 71(0.8) | |
| Tl ²⁰⁴ 3.779y | Pb ^{204m} 66.9m Hg ²⁰⁴ S Pb ²⁰⁴ | β⁻ EC (2.58) Hg x-rays 10(0.8), 69(0.4), 71(0.7), 80(0.3) IT γ | 763 (97.42) Hg x-rays 10(0.8), 69(0.4), 71(0.7), 80(0.3) 375 (94.11), 899 (99.2), 912 (91.1) Pb x-rays 11(4.9), 73(2.8), 75(4.36), 85(1.94) |

Pb-208 (S), Tl-208, Po-212, Bi-212, Pb-212, Po-216, Rn-220, Ra-224, Th-228, Ac-228, Ra-228, Th-232 are in the Thorium-232 decay chain.

Pb-206 (S), Tl-206, Po-210, Bi-210, Pb-210, Tl-210, Po-214, Bi-214, Pb-214, At-218, Po-218, Rn-222, Ra-226, Th-230, U-234, Pa-234, Pa-234m, Th-234, U-238 are in the Uranium-238 decay chain.

Bi-209 (S), Tl-209, Pb-209, Po-213, Bi-213, At-217, Fr-221, Ac-225, Ra-225, Th-229, U-233, Pa-233, U-237, Np-237, Am-241, Pu-241 are in the Neptunium (4n+1) decay chain.

Pb-207 (S), Tl-207, Po-211, Bi-211, Pb-211, At-215, Po-215, Rn-219, Ra-223, Fr-223, Th-227, Ac-227, Pa-231, Th-231, U-235 are in the Actinium (4n+3) decay chain.

| | | | |
|-------------------------------|-------------------|----------------------------------|---|
| Pu ²³⁶ 2.851y | U ²³² | α γ U x-rays | 5614 (0.2), 5722 (31.8), 5770 (68.1) av. 61 (0.08) 14 (13) |
| U ²³² 68.81y | Th ²²⁸ | α | 5414 (100) |
| Pu ²⁴² 3.742E5y | U ²³⁸ | α U x-rays | 4984 (100) 14 (9.1) |
| Cm ²⁴² 162.85d | Pu ²³⁸ | α γ Pu x-rays | 6070 (25.9), 6113 (74.1) av. 59 (0.04) 14 (11.5) |
| Pu ²³⁸ 87.84y | U ²³⁴ | α γ U x-rays | 5358 (0.1), 5456 (29.0), 5499 (70.9) 43 (0.04), 100 (0.007), 153 (0.0009) 14 (4.0) |
| Am ²⁴³ 7.388E3y | Np ²³⁹ | α γ Np x-rays | 5181 (1), 5234 (10.6), 5275 (87.9) 43 (5.5), 75 (66), 118 (0.55) 14 (39) |
| Np ²³⁹ 2.3565d | Pu ²³⁹ | β ⁻ γ Pu x-rays | 330 (35.7), 391 (7.1), 436 (52) 106 (22.7), 228 (10.7), 278 (14.1) 14 (62), 100 (14.7), 104 (23.7), 117 (11.1) |
| Pu ²³⁹ 24,125y | U ²³⁵ | α γ U x-rays | 5105(11.5), 5143(15.1), 5155(73.3) 52(0.02), 129(0.0062), 375(0.0015), 414 (0.0015) 14 (4.4) |

| | | |
|------------------------------|-------------------|--|
| Cm ²⁴⁴ 18.11y | Pu ²⁴⁰ | α 5763 (23.6), 5805 (76.4) γ av. 57 (0.03) Pu x-rays 14 (10.3) |
| Pu ²⁴⁰ 6567.1y | U ²³⁶ | α 5123 (26.4), 5168 (73.5) γ av. 54 (0.05) U x-rays 14(11) |
| Bk ²⁴⁹ 320d | Cf ²⁴⁹ | β⁻ 124 (100) |
| Cf ²⁴⁹ 350.6y | Cm ²⁴⁵ | α 5760(3.66), 5814(84.4), 5946(4) γ 253 (2.7), 333 (15.5), 388 (66) Cm x-rays 15(30), 105 (2.19), 109 (3.5), 123 (1.66) |
| Cm ²⁴⁵ 8.56E3y | Pu ²⁴¹ | α 5392(5.0), 5451(93.2), 5580(0.8) Pu x-rays 42 (38.2), 133 (34.7), 175 (61) |
| Cf ²⁵² 2.639y | Cm ²⁴⁸ | α 5977(0.2), 6076(15.2), 6118(81.6) γ av. 68 (0.03) Cm x-rays 15 (7.3) spontaneous fission (3) |
| Cm ²⁴⁸ 333.5d | Pu ²⁴⁴ | α 5162 (91.61) spontaneous fission (8.39) |
| Pu ²⁴⁴ 7.93E7y | U ²⁴⁰ | α 4666 (100) spontaneous fission (0.121) |
| U ²⁴⁰ 14.1h | Np ²⁴⁰ | β⁻ 440 (100) γ 44 (1.65) Np x-rays 14 (4.4) |
| Np ²⁴⁰ 7.4m | Pu ²⁴⁰ | β⁻ 2188 (100) |

Thorium-232 Decay Chain (including Thoron Progeny)

1st Progeny kev and % abundance

| | | | |
|-------------------------------|-------------------|----------------|--|
| Th ²³² 1.41E10y | Ra ²²⁸ | α | 3830(0.2), 3953 (23), 4010 (77) |
| | | γ | 59 (0.19), 125 (0.04) |
| | | Ra x-rays | 12 (8.4) |
| Ra ²²⁸ 5.75y | Ac ²²⁸ | β ⁻ | 39 (100) |
| Ac ²²⁸ 6.13h | Th ²²⁸ | β ⁻ | 606 (8), 1168 (32), 1741 (12) |
| | | γ | 338(11.4), 911(27.7), 969(16.6) |
| Th ²²⁸ 1.91y | Ra ²²⁴ | Th x-rays | 13 (39), 90 (2.1), 93 (3.5), 105 (1.6) |
| | | α | 5212(0.4), 5341(26.7), 5423(72.7) |
| | | γ | 84 (1.2), 132 (0.12), 216 (0.24) |
| Ra ²²⁴ 3.62d | Rn ²²⁰ | Ra x-rays | 12 (9.6) |
| | | α | 5449 (4.9), 5686 (95.1) |
| | | γ | 241 (3.95) |
| | | Rn x-rays | 12(0.4), 81 (0.126), 84 (0.209) |

Rn²²⁰ is “thoron” gas, usually included with “radon” gas

| | | | |
|-----------------------------|-------------------|----------------|---------------------------------------|
| Rn ²²⁰ 56s | Po ²¹⁶ | α | 6288 (99.9), 5747 (0.1) |
| Po ²¹⁶ 0.15s | Pb ²¹² | γ | av. 550 (0.1) |
| Pb ²¹² 10.64h | Bi ²¹² | α | 6779 (99.998) |
| | | β ⁻ | 158(5.22), 334 (85.1), 573 (9.9) |
| | | γ | 115 (0.6), 239 (44.6), 300 (3.4) |
| | | Bi x-rays | 11 (15.5), 75 (10.7), 77 (18), 87 (8) |

Bi²¹² decays 64.7% of the time by β⁻ to Po²¹² and 35.93% by α to Tl²⁰⁸

| | | |
|----------------------------|--|---|
| Bi ²¹² 60.6m | Tl ²⁰⁸ Po ²¹² | α 5767 (0.6), 6050 (25.2), 6090 (9.6) β⁻ 625 (3.4), 1519 (8), 2426 (48.4) γ 727 (11.8), 785 (1.97), 1621 (2.75) Tl x-rays 10 (7.7) |
| Tl ²⁰⁸ 3.05m | Pb ²⁰⁸ S | β⁻ 1283(23.2), 1517(22.7), 1794(49.3) γ 511 (21.6), 583 (84.2), 860(12.46), 2614 (99.8) Pb x-rays 11 (2.9), 73 (2.0), 75 (3.4), 85 (1.5) |
| Po ²¹² 304ns | Pb ²⁰⁸ S | α 8785 (100) |

Pb²⁰⁸ is Stable

Uranium-238 Decay Chain (including Radon Progeny)

1st Progeny kev and % abundance

| | | | |
|---|-------------|--------------------|--|
| U^{238} | Th^{234} | α | 4039(0.2), 4147(23.4), 4196(77.4) |
| 4.47E9 y | | γ | av. 66 (0.1) |
| Th^{234} | Pa^{234m} | Th x-rays | 13 (8.8) |
| 24.1d | | β^- | 76 (2), 96 (25.3), 189 (72.5) |
| | | γ | 63 (3.8), 92 (2.7), 93 (2.7) |
| | | Pa x-rays | 13 (9.6) |
| Pa^{234m} decays 99.87% of the time by β^- to U^{234} and 0.13% of the time by IT to Pa^{234} | | | |
| Pa^{234m} | U^{234} | β^- | 1236(0.7), 1471(0.6), 2281(98.6) |
| 1.17m | | γ | 766 (0.2), 926 (0.4), 1001 (0.6) |
| | | U x-rays | 14(0.44), 95(0.115), 98(0.187) |
| Pa^{234} | Pa^{234} | IT | |
| 6.70h | U^{234} | β^- | 484 (35), 654 (0.6), 1183(10) |
| | | γ | 131 (20.4), 882 (24), 946 (12) |
| | | U x-rays | 14(144), 95(15.7), 98(25.4), 111(11.8) |
| U^{234} | Th^{230} | α | 4605(0.2), 4724(27.4), 4776(72.4) |
| 2.45E5y | | γ | 53 (0.118), 121 (0.04) |
| Th^{230} | Ra^{226} | α | 4476(0.12), 4621(23.4), 4688(76.3) |
| 7.7E4y | | | |
| Ra^{226} | Rn^{222} | α | 4602 (5.6), 4785 (94.4) |
| 1600y | | γ | 186 (3.28) |
| | | Rn x-rays | 12(0.4), 81(0.18), 84(0.3), 95(0.14) |
| Rn^{222} is “radon” gas, usually included with “thoron” gas | | | |
| Rn^{222} | Po^{218} | α | 5490 (99.92), 4986 (0.08) |
| 3.82d | | γ | av. 512 (0.08) |
| Po^{218} decays 99.98% of the time by α to Pb^{214} and 0.02% of the time by β^- to At^{218} | | | |
| Po^{218} | Pb^{214} | α | 6003 (99.98) |
| 3.05 | At^{218} | β^- | 330 (0.02) |

| | | | |
|---|-------------------|-----------|--|
| At ²¹⁸ | Bi ²¹⁴ | α | 6650 (6), 6700 |
| 2s | | | |
| Pb ²¹⁴ | Bi ²¹⁴ | β^- | 672(48), 729 (42.5), 1024 (6.3) |
| 26.8m | | γ | 242(7.49), 295(19.2), 352(37.2) |
| | | | Bi x-rays 11(13.5), 75(6.2), 77(10.5), 87(4.7) |
| Bi ²¹⁴ decays 99.979% of the time by β^- to Po ²¹⁴ and 0.021% of the time by α to Tl ²¹⁰ | | | |
| Bi ²¹⁴ | Po ²¹⁰ | β^- | 1505(17.7), 1540(17.9), 3270(17.2) |
| 19.9m | | γ | 609(46.3), 1120(15.1), 1764(15.8) |
| | | | Po x-rays 11(0.5), 77(0.36), 79(06), 90(0.3) |
| Po ²¹⁴ | Pb ²¹⁰ | α | 7687 (99.989), 6892 (0.01) |
| 146us | | γ | 797 (0.013) |
| Tl ²¹⁰ | Pb ²¹⁰ | β^- | 1320 (25), 1870 (56), 2340 (19) |
| 1.30m | | γ | 298 (79), 800 (99), 1310(21) |
| | | | Pb x-rays 11(13), 73(2.5), 75(4.3), 85(1.9) |
| Pb ²¹⁰ | Bi ²¹⁰ | β^- | 17 (80.2), 63 (19.8) |
| 22.3y | | γ | 47 (4.05) |
| | | | Bi x-rays 11 (24.3) |
| Bi ²¹⁰ decays ~100% of the time by β^- to Po ²¹⁰ and 0.000013% of the time by α to Tl ²⁰⁶ | | | |
| Bi ²¹⁰ | Po ²¹⁰ | β^- | 1161 (99.9998) |
| 5.01d | Tl ²⁰⁶ | α | 4650 (0.00007), 4690 (00005) |
| Po ²¹⁰ | Pb ²⁰⁶ | α | 5350(99.9989) |
| 138.4d | S | | |
| Tl ²⁰⁶ | Pb ²⁰⁶ | β^- | 1520 (100) |
| 4.19m | S | | |

Pb²⁰⁶ is Stable

Neptunium-232 Decay Chain

1st Progeny kev and % abundance

Pu²⁴¹ decays ~100% of the time by β^- to Am²⁴¹ and 0.0023% of the time by α to U²³⁷

| | | | |
|---|--|--|---|
| Pu ²⁴¹ 14.4y Am ²⁴¹ 432.2y | Am ²⁴¹ U ²³⁷ Np ²³⁷ | β^- α α γ Np x-rays | 21 (~100) 4850 (0.0003), 4900 (0.0019) 5440 (13), 5490 (85) 26 (2.4), 33 (0.1), 59.5 (36) 14 (43) |
| Np ²³⁷ 6.75d | Pa ²³³ | β^- γ | 248 (96) 30 (14), 86 (14), 208 (22) |
| Pa ²³³ 27.0d | U ²³³ | β^- γ | Pa x-rays 13.3 (59), 92 (1.58), 108 (1.2) 145 (37), 257 (58), 568 (5) 75 (1.2), 87 (1.9), 311 (49) |
| U ²³³ 1.592E5y | Th ²²⁹ | α | U x-rays 14 (49), 96 (28), 111 (8) 4780 (15), 4820 (83) |
| Th ²²⁹ 7.34E3y | Ra ²²⁵ | β^- | Th x-rays 13 (3.9) 4840 (58), 4900 (11), 5050 (7) 31 (4), 137 (2), 211 (3.3) |
| Ra ²²⁵ 14.8d | Ac ²²⁵ | β^- | Ra x-rays 12 (81), 85 (16), 100 (12) 320 (100) |
| Ac ²²⁵ 10.0y | Fr ²²¹ | γ | 40 (31) |
| Fr ²²¹ 4.8m | At ²¹⁷ | α | 5935 (100) 6126(15), 6242(1.4), 6340(83.4) |
| At ²¹⁷ 0.0323s | Bi ²¹³ | γ | 100 (0.2), 218 (12.5), 412 (0.1) At x-rays 11 (2.3), 80 (2), 92 (0.6) 7066 (99.9) |
| Bi ²¹³ decays 97.84% of the time by β^- to Po ²¹³ and 2.16% of the time by α to Tl ²⁰⁹ | | | 595 (004) |

| | | | |
|-----------------------------|-------------------|-----------|---------------------------------|
| Bi ²¹³ | Po ²¹³ | β^- | 320 (1.06), 980 (32), 1420(64) |
| 45.65m | | γ | 293 (0.7), 440 (28), 1100 (0.5) |
| | | Po x-rays | 11 (1.8), 78 (3.4), 90 (1) |
| Po ²¹³ | Tl ²⁰⁹ | α | 5549 (0.16), 5870 (2) |
| 4.2E-6s | Pb ²⁰⁹ | α | 8377 (~100) |
| Tl ²⁰⁹ | Pb ²⁰⁹ | β^- | 1825 (100) |
| 2.20m | | γ | 117(77), 465(96.6), 1567(99.7) |
| Pb ²⁰⁹ | Bi ²⁰⁹ | Pb x-rays | 10.6 (8.7), 74 (16), 85 (4.4) |
| 3.253h | S | β^- | 645 (100) |
| Bi ²⁰⁹ is Stable | | | |

Actinium Decay Chain (4n + 3)

1st Progeny

kev and % abundance

| | | | |
|---|------------|-----------|----------------------------------|
| U^{235} | Th^{231} | α | 4370 (18), 4400 (57), 4580 (8) |
| 7.08E8y | | γ | 143 (11), 185 (54), 204 (5) |
| Th^{231} | Pa^{231} | β^- | 140 (45), 220 (15), 305 (40) |
| 25.5h | | γ | 26 (2), 84 (10) |
| Pa^{231} | Ac^{227} | α | 4950 (22), 5010 (24), 5020(23) |
| 3.48E4y | | γ | 27 (6), 29 (6) |
| Ac^{227} decays 98.62% of the time by β^- to Th^{227} and 1.38% of the time by α to Fr^{223} | | | |
| Ac^{227} | Th^{227} | β^- | 43 (98.6) |
| 21.77y | | γ | 70 (0.08) |
| | Fr^{223} | α | 4860 (0.18), 4950 (1.2) |
| Th^{227} | Ra^{223} | α | 5760 (21), 5980 (24), 6040 (23) |
| 18.72d | | γ | 50 (8), 237 (15), 310 (8) |
| Fr^{223} | Ra^{223} | β^- | 1150 (~100) |
| 21.8m | | γ | 50 (8), 80 (13), 234 (4) |
| Ra^{223} | Rn^{219} | α | 5610 (26), 5710 (54), 5750 (9) |
| 11.435d | | γ | 33 (6), 149 (10), 270 (10) |
| Rn^{219} | Po^{215} | α | 6420 (8), 6550 (11), 6820 (81) |
| 3.96s | | γ | 272 (9), 401 (5) |
| Po^{215} decays ~100% of the time by α to Pb^{211} and 0.00023% of the time by β^- to At^{215} | | | |
| Po^{215} | Pb^{211} | α | 7380 (~100) |
| 1.778ms | At^{215} | β^- | 740 (0.00023) |
| At^{215} | Bi^{211} | α | 8010 (100) |
| 0.1ms | | | |
| Pb^{211} | Bi^{211} | β^- | 290(1.4), 560 (9.4), 1390 (87.5) |
| 36.1m | | γ | 405 (3.4), 427 (1.8), 832 (3.4) |
| Bi^{211} decays 99.73% of the time by α to Tl^{207} and 0.273% of the time by β^- to Po^{211} | | | |

| | | | |
|-------------------|-------------------|-----------|----------------------|
| Bi^{211} | Tl^{207} | α | 6280 (16), 6620 (84) |
| 2.13m | | γ | 351 (14) |
| | Po^{211} | β^- | 600 (0.28) |
| Po^{211} | Pb^{207} | α | 7450 (99) |
| 0.516s | S | γ | 570 (0.5), 900 (0.5) |
| Tl^{207} | Pb^{207} | β^- | 1440 (99.8) |
| 4.77m | S | γ | 897 (0.16) |

Pb^{207} is Stable

Ci / g = 3.578E5 / (T_{1/2} in years x atomic mass)

GBq / g = 1.324E7 / (T_{1/2} in years x atomic mass)

| | Half-Life | Ci/g | Rem/hr / Ci | Sv/hr / GBq |
|---------|------------------|----------------|--------------------|--------------------|
| | | @ 30 cm | GBq/g | @ 30cm |
| Ac-227 | 21.77y | 72.40 | N/A | 2.68E3 |
| Ac-228 | 6.15h | 2.24E6 | 2.82 | 8.29E7 |
| Ag-110 | 24.6s | 4.17E9 | 0.18 | 1.54E11 |
| Ag-110m | 249.79d | 13.03 | 14.66 | 482 |
| Ag-111 | 7.45d | 65.79 | 0.16 | 2.43E3 |
| Al-26 | 7.3E5y | 0.019 | 16.6 | 0.699 |
| Am-241 | 432.7y | 3.43 | 0.19 | 127 |
| Am-242 | 16.02h | 8.08E5 | 0.23 | 2.99E7 |
| Am-243 | 7370y | 0.20 | 0.23 | 7.40 |
| Ar-37 | 35.04d | 1.01E5 | N/A | 3.73E6 |
| Ar-39 | 269.0y | 34.14 | N/A | 1.26E3 |
| Ar-41 | 1.82h | 4.20E7 | 7.73 | 1.55E9 |
| Ar-42 | 32.90y | 259.20 | N/A | 9.59E3 |
| As-74 | 17.8d | 9.91E4 | 0.586 | 3.67E6 |
| At-215 | 0.100us | 5.25E14 | N/A | 1.94E16 |
| At-216 | 300us | 1.74E14 | N/A | 6.44E15 |
| At-218 | 1.6s | 3.23E10 | N/A | 1.20E12 |
| Au-198 | 2.695d | 2.12E10 | 0.279 | 7.84E11 |
| Ba-131 | 11.5d | 8.68E4 | 2.15 | 3.21E6 |
| Ba-133 | 10.52y | 255.90 | 2.22 | 9.47E3 |
| Ba-137m | 2.552m | 5.37E8 | 4.44 | 1.99E10 |
| Ba-139 | 83.06m | 1.63E7 | 0.173 | 6.03E8 |
| Ba-140 | 12.75d | 7.32E4 | 0.871 | 2.71E6 |
| Ba-141 | 18.27m | 7.31E7 | 2.4 | 2.70E9 |
| Ba-142 | 10.6m | 1.25E8 | 1.01 | 4.63E9 |
| Be-7 | 53.28d | 3.50E5 | 0.38 | 1.30E7 |
| Be-10 | 1.51E6y | 0.024 | N/A | 0.875 |
| Bi-210 | 5.01d | 1.24E5 | N/A | 4.59E6 |
| Bi-210m | 3.04E6y | 5.61E-4 | 2.124 | 0.0207 |

| | Half-Life | Ci/g | Rem/hr / Ci | GBq/g | Sv/hr / GBq |
|--------|------------------|-------------|--------------------|--------------|--------------------|
| | | | @ 30 cm | | @ 30cm |
| Bi-211 | 2.14m | 4.17E8 | 0.273 | 1.54E10 | 7.39E-5 |
| Bi-212 | 60.6m | 1.47E7 | N/A | 5.44E8 | N/A |
| Bi-213 | 45.59m | 1.94E7 | 0.739 | 7.17E8 | 2.00E-4 |
| Bi-214 | 19.9m | 4.41E7 | 9.31 | 1.63E9 | 2.52E-3 |
| Bk-249 | 320d | 1.64E3 | N/A | 6.07E4 | N/A |
| Br-82 | 17.68m | 1.33E8 | 2.15 | 4.92E9 | 5.82E-4 |
| Br-84 | 31.8m | 7.05E7 | 0.172 | 2.61E9 | 4.66E-5 |
| C-11 | 1223s | 8.38E8 | 6.815 | 3.10E10 | 1.84E-3 |
| C-14 | 5730y | 4.46 | N/A | 165 | N/A |
| Ca-41 | 1.03E5y | 0.085 | N/A | 3.14 | N/A |
| Ca-47 | 4.536d | 6.13E5 | 0.198 | 2.27E7 | 5.36E-5 |
| Cd-109 | 1.264y | 2.6E3 | 0.528 | 9.62E4 | 1.43E-4 |
| Cd-113 | 7.70E15y | 4.12E-13 | N/A | 1.52E-11 | N/A |
| Cd-118 | 50.3m | 3.17E7 | N/A | 1.17E9 | N/A |
| Ce-141 | 32.5d | 2.85E4 | 0.422 | 1.06E6 | 1.14E-4 |
| Ce-143 | 33.1h | 6.63E5 | 1.19 | 2.45E7 | 3.22E-4 |
| Cf-249 | 351y | 4.09 | 1.98 | 151 | 5.35E-4 |
| Cf-252 | 2.638y | 538 | N/A | 1.99E4 | N/A |
| Cf-255 | 85.0m | 8.67E6 | N/A | 3.21E8 | N/A |
| Cf-256 | 12.3m | 5.97E7 | N/A | 2.21E9 | N/A |
| Cl-36 | 3.01E5y | 0.033 | N/A | 1.22 | N/A |
| Cl-38 | 37.24m | 1.33E8 | 8.92 | 4.92E9 | 2.41E-3 |
| Cm-242 | 162.8d | 3.31E3 | N/A | 1.22E5 | N/A |
| Cm-243 | 29.1y | 50.59 | 0.675 | 1.87E3 | 1.83E-4 |
| Cm-244 | 18.1y | 81.0 | N/A | 3.00E3 | N/A |
| Cm-245 | 8500y | 0.17 | 0.325 | 6.36 | 8.80E-5 |
| Cm-247 | 1.56E7y | 9.28E-5 | 1.87 | 3.43E-3 | 5.06E-4 |
| Co-56 | 77.3d | 3.02E4 | 21.36 | 1.12E6 | 5.77E-3 |
| Co-57 | 271.8d | 8.43E3 | 0.713 | 3.12E5 | 4.54E-4 |
| Co-58 | 70.88d | 3.18E4 | 6.81 | 1.18E6 | 1.84E-3 |
| Co-60 | 5.271y | 1.13E3 | 15.19 | 4.18E4 | 4.11E-3 |

| | Half-Life | Ci/g | Rem/hr / Ci @ 30 cm | GBq/g | Sv/hr / GBq @ 30cm |
|---------|------------------|-------------|--------------------------------|--------------|-------------------------------|
| Cr-51 | 27.70d | 9.24E4 | 0.207 | 3.42E6 | 5.61E-5 |
| Cs-134 | 2.0648y | 1.29E3 | 10.25 | 4.79E4 | 2.77E-3 |
| Cs-134m | 2.903h | 8.06E6 | 0.0986 | 2.98E8 | 2.67E-5 |
| Cs-135 | 2.30E6y | 1.15E-3 | N/A | 0.0427 | N/A |
| Cs-136 | 13.16d | 7.30E4 | 6.85 | 2.70E6 | 1.85E-3 |
| Cs-137 | 30.17y | 86.6 | See Ba137m | 3.20E3 | N/A |
| Cs-138 | 33.41m | 4.08E7 | 2.31 | 1.51E9 | 6.25E-4 |
| Cu-61 | 3.333h | 1.54E7 | 1.05 | 5.71E8 | 2.84E-4 |
| Cu-62 | 9.74m | 3.11E8 | 7.85 | 3.39E7 | 2.12E-3 |
| Cu-64 | 12.7h | 3.86E6 | 1.228 | 1.43E8 | 3.33E-4 |
| Dy-154 | 3.00E6y | 7.75E-4 | N/A | 0.0287 | N/A |
| Dy-165 | 2.334h | 8.14E6 | 0.0918 | 3.01E8 | 2.49E-5 |
| Es-253 | 20.47d | 2.52E4 | N/A | 9.32E5 | N/A |
| Es-256 | 25.4m | 2.89E7 | N/A | 1.07E9 | N/A |
| Eu-152 | 13.537y | 174.0 | 5.82 | 6.44E3 | 1.58E-3 |
| Eu-154 | 8.589y | 270.6 | 7.06 | 1.00E4 | 1.91E-3 |
| Eu-155 | 4.7611y | 485.1 | 0.319 | 1.79E4 | 8.64E-5 |
| Eu-156 | 15.19d | 5.51E4 | 1.3 | 2.04E6 | 3.52E-4 |
| F-18 | 1.830h | 9.52E7 | 7.72 | 3.52E9 | 2.09E-3 |
| Fe-55 | 2.73y | 2.38E3 | N/A | 8.81E4 | N/A |
| Fe-59 | 44.51d | 4.97E4 | 7.34 | 1.84E6 | 1.98E-3 |
| Fe-60 | 1.50E6y | 3.98E-3 | N/A | 0.147 | N/A |
| Fm-256 | 157.6m | 4.66E6 | N/A | 1.72E8 | N/A |
| Fr-219 | 20.0ms | 2.58E12 | N/A | 9.53E13 | N/A |
| Fr-221 | 4.9m | 1.74E8 | 0.163 | 6.43E9 | 4.41E-5 |
| Fr-223 | 21.8m | 3.87E7 | 0.0952 | 1.43E9 | 2.58E-5 |
| Ga-67 | 3.2612d | 5.98E5 | 0.9381 | 2.21E7 | 2.54E-4 |
| Gd-148 | 75y | 32.2 | N/A | 1.19E3 | N/A |
| Gd-150 | 1.79E6y | 1.33E-3 | N/A | 0.0493 | N/A |
| Gd-152 | 1.08E14y | 2.18E-11 | N/A | 8.07E-10 | N/A |
| Ge-68 | 270.8d | 7.09E3 | N/A | 2.62E5 | N/A |

| | | | Rem/hr / Ci | | Sv/hr / GBq |
|---------|------------------|-------------|--------------------|--------------|--------------------|
| | Half-Life | Ci/g | @ 30 cm | GBq/g | @ 30cm |
| H-3 | 12.3y | 9.70E3 | N/A | 3.59E5 | N/A |
| Hf-174 | 2.00E15y | 1.03E-12 | N/A | 3.81E-11 | N/A |
| Hg-203 | 46.612d | 1.38E4 | 1.29 | 5.11E5 | 3.49E-4 |
| Ho-163 | 4.57E3y | 0.48 | N/A | 17.8 | N/A |
| Ho-166 | 26.8h | 7.05E5 | 0.1164 | 2.61E7 | 3.15E-5 |
| Ho-166m | 1200y | 1.80 | 5.39 | 66.5 | 1.46E-3 |
| I-123 | 13.27h | 1.92E6 | 0.796 | 7.11E7 | 2.15E-4 |
| I-124 | 4.176d | 2.52E5 | 5.53 | 9.34E6 | 1.50E-3 |
| I-125 | 60.1d | 1.74E4 | 1.664 | 6.44E5 | 4.50E-4 |
| I-126 | 12.93d | 7.97E4 | 4.34 | 2.95E6 | 1.17E-3 |
| I-129 | 1.57E7y | 1.77E-4 | 0.736 | 6.55E-3 | 1.99E-4 |
| I-130 | 12.36h | 1.55E6 | 4.76 | 5.74E7 | 1.29E-3 |
| I-131 | 8.040d | 1.24E5 | 3.14 | 4.59E6 | 8.49E-4 |
| I-132 | 2.295h | 1.04E7 | 5.17 | 3.83E8 | 1.40E-3 |
| I-133 | 20.8h | 1.13E6 | 4.54 | 4.18E7 | 1.23E-3 |
| I-134 | 52.6m | 2.67E7 | 17.47 | 9.88E8 | 4.72E-3 |
| I-135 | 6.57h | 3.53E6 | 9.57 | 1.31E8 | 2.59E-3 |
| In-111 | 2.8047d | 4.20E5 | 3.717 | 1.55E7 | 1.01E-3 |
| In-113m | 1.6582h | 1.69E7 | 1.53 | 6.25E8 | 4.14E-4 |
| In-115 | 4.41E14y | 7.06E-12 | N/A | 2.61E-10 | N/A |
| Ir-192 | 73.83d | 9.21E3 | 6.56 | 3.41E5 | 1.77E-3 |
| K-40 | 1.28E9y | 6.99E-6 | 0.91 | 2.59E-4 | 2.46E-4 |
| K-42 | 12.36h | 6.04E6 | 1.4 | 2.23E8 | 3.78E-4 |
| K-43 | 22.3h | 3.27E6 | 5.6 | 1.21E8 | 1.51E-3 |
| Kr-85 | 10.73y | 392.0 | 0.02 | 1.45E4 | 5.40E-6 |
| Kr-85m | 4.48h | 8.24E6 | 0.96 | 3.05E8 | 2.60E-4 |
| Kr-87 | 76.3m | 2.84E7 | 3.18 | 1.05E9 | 8.61E-4 |
| Kr-88 | 2.84h | 1.26E7 | 8.9 | 4.64E8 | 2.41E-3 |
| Kr-89 | 3.15m | 6.71E8 | 3.96 | 2.48E10 | 1.07E-3 |
| La-140 | 1.678d | 5.56E5 | 13.61 | 2.06E7 | 3.68E-3 |
| La-142 | 91.1m | 1.46E7 | 0.675 | 5.38E8 | 1.83E-4 |

| | Half-Life | Ci/g | Rem/hr / Ci | GBq/g | Sv/hr / GBq |
|---------|------------------|-------------|--------------------|--------------|--------------------|
| | | | @ 30 cm | | @ 30cm |
| Lu-177 | 6.73d | 1.10E5 | 0.170 | 4.06E6 | 4.61E-5 |
| Mn-52 | 5.591d | 4.49E5 | 18.6 | 1.66E7 | 5.03E-3 |
| Mn-52m | 21.2m | 1.72E8 | 1.48 | 6.35E9 | 4.01E-4 |
| Mn-53 | 3.74E6y | 1.81E-3 | N/A | 0.0669 | N/A |
| Mn-54 | 312.2d | 7.75E3 | 5.67 | 2.87E5 | 1.53E-3 |
| Mn-56 | 2.578h | 2.17E7 | 10.24 | 8.03E8 | 2.77E-3 |
| Mo-99 | 67h | 4.80E5 | 1.25 | 1.78E7 | 3.38E-4 |
| N-13 | 9.965m | 1.45E9 | 6.814 | 5.37E10 | 1.84E-3 |
| N-16 | 7.13s | 9.89E10 | 16.57 | 3.66E12 | 4.48E-3 |
| Na-22 | 2.605y | 6.24E3 | 14.85 | 2.31E5 | 4.01E-3 |
| Na-24 | 14.96h | 8.73E6 | 20.55 | 3.23E8 | 5.55E-3 |
| Nb-94 | 2.03E5y | 0.19 | 10.20 | 6.94 | 2.76E-3 |
| Nb-95 | 34.975d | 3.93E4 | 4.74 | 1.46E6 | 1.28E-3 |
| Nd-144 | 2.29E15y | 1.09E-12 | N/A | 4.02E-11 | N/A |
| Ni-57 | 35.6h | 1.54E6 | 12 | 5.70E7 | 3.24E-3 |
| Ni-59 | 7.60E4y | 0.080 | 12.5 | 2.95 | 3.38E-3 |
| Ni-63 | 101y | 56.23 | N/A | 2.08E3 | N/A |
| Ni-65 | 2.52h | 1.91E7 | 3.4 | 7.07E8 | 9.19E-4 |
| Ni-66 | 54.6h | 8.71E5 | N/A | 3.22E7 | N/A |
| Np-237 | 2.14E6y | 7.05E-4 | 0.0868 | 0.0261 | 2.35E-5 |
| Np-238 | 2.117d | 2.59E5 | 0.018 | 9.59E6 | 4.87E-6 |
| Np-239 | 2.355d | 2.32E5 | 0.594 | 8.58E6 | 1.61E-4 |
| Np-240 | 61.9m | 1.27E7 | 0.863 | 4.68E8 | 2.34E-4 |
| O-15 | 122.2s | 6.15E9 | 7.98 | 2.29E11 | 2.16E-3 |
| Os-186 | 2E15y | 9.62E-13 | 0.613 | 3.56E-11 | 1.66E-4 |
| P-32 | 14.28d | 2.86E5 | N/A | 1.06E7 | N/A |
| P-33 | 25.34d | 1.56E5 | N/A | 5.78E6 | N/A |
| Pa-231 | 3.28E4y | 0.047 | 0.104 | 1.75 | 2.81E-5 |
| Pa-233 | 26.967d | 2.08E4 | 1.27 | 7.69E5 | 3.44E-4 |
| Pa-234 | 6.69h | 2.00E6 | 7.03 | 7.40E7 | 1.90E-3 |
| Pa-234m | 1.17m | 6.86E8 | 0.05 | 2.54E10 | 1.35E-5 |

| | Half-Life | Ci/g | Rem/hr / Ci | Sv/hr / GBq |
|---------|------------------|-------------|--------------------|--------------------|
| | | | @ 30 cm | @ 30cm |
| Pb-209 | 3.253h | 4.61E6 | N/A | 1.71E8 |
| Pb-210 | 22.3y | 76.4 | 0.0203 | 2.83E3 |
| Pb-211 | 36.1m | 2.47E7 | 0.248 | 9.14E8 |
| Pb-212 | 10.64h | 1.39E6 | 0.732 | 5.14E7 |
| Pb-214 | 27m | 3.25E7 | 1.155 | 1.20E9 |
| Pd-107 | 6.50E6y | 5.15E-4 | N/A | 0.0191 |
| Pm-147 | 2.6234y | 928.3 | 3.15E-5 | 3.43E4 |
| Pm-149 | 53.08h | 3.97E5 | 0.0532 | 1.47E7 |
| Pm-151 | 4.12m | 7.31E5 | 1.2 | 2.71E7 |
| Po-210 | 138.38d | 4.49E3 | N/A | 1.66E5 |
| Po-212 | 304ns | 1.78E17 | N/A | 6.59E18 |
| Po-214 | 164us | 3.22E14 | 6.71E-4 | 1.19E16 |
| Po-216 | 145ms | 3.60E11 | 9.95E-5 | 1.33E13 |
| Po-218 | 3.10m | 2.78E8 | N/A | 1.03E10 |
| Pr-142m | 14.6m | 9.08E7 | N/A | 3.36E9 |
| Pt-190 | 6.50E11y | 2.90E-9 | N/A | 1.07E-7 |
| Pt-202 | 44.0h | 3.53E5 | N/A | 1.30E7 |
| Pu-236 | 2.87y | 528 | N/A | 1.95E4 |
| Pu-238 | 87.7y | 17.1 | 0.877 | 633 |
| Pu-239 | 2.41E4y | 0.062 | 0.335 | 2.30 |
| Pu-240 | 6560y | 0.227 | N/A | 8.40 |
| Pu-241 | 14.4y | 103 | N/A | 3.81E3 |
| Pu-242 | 3.75E5y | 3.94E-3 | N/A | 0.146 |
| Ra-223 | 11.435d | 5.12E4 | 0.37 | 1.89E6 |
| Ra-224 | 3.66d | 1.59E5 | 0.054 | 5.88E6 |
| Ra-225 | 14.9d | 3.90E4 | 0.07 | 1.44E6 |
| Ra-226 | 1600y | 0.99 | 0.045 | 36.6 |
| Ra-228 | 5.76y | 272 | N/A | 1.01E4 |
| Rb-81 | 4.576h | 8.47E6 | 3.628 | 3.13E8 |
| Rb-82 | 1.273m | 1.80E9 | 7.452 | 6.67E10 |
| Rb-83 | 86.2d | 1.83E4 | 3.135 | 6.76E5 |

| | Half-Life | Ci/g | Rem/hr / Ci | GBq/g | Sv/hr / GBq |
|--------|------------------|-------------|--------------------|--------------|--------------------|
| | | | @ 30 cm | | @ 30cm |
| Rb-87 | 4.75E10y | 8.67E-8 | N/A | 3.21E-6 | N/A |
| Rb-88 | 17.7m | 1.21E8 | 3.58 | 4.48E9 | 9.68E-4 |
| Rb-89 | 15.4m | 1.37E8 | 12.17 | 5.07E9 | 3.29E-3 |
| Re-187 | 4.35E10y | 4.40E-8 | N/A | 1.63E-6 | N/A |
| Re-188 | 16.98h | 9.82E5 | 0.2096 | 3.63E7 | 5.67E-5 |
| Rh-105 | 35.36h | 8.45E5 | 0.462 | 3.13E7 | 1.25E-4 |
| Rh-106 | 29.8s | 3.58E9 | 0.644 | 1.32E11 | 1.74E-4 |
| Rn-212 | 23.9m | 3.71E7 | N/A | 1.37E9 | N/A |
| Rn-216 | 45.0us | 1.16E15 | N/A | 4.30E16 | N/A |
| Rn-219 | 3.96s | 1.30E10 | 0.329 | 4.81E11 | 8.91E-5 |
| Rn-220 | 55.6s | 9.21E8 | 3.99E-3 | 3.41E10 | 1.08E-6 |
| Rn-222 | 3.8235d | 1.54E5 | 3.03E-3 | 5.70E6 | 8.19E-7 |
| Ru-97 | 2.9d | 4.65E5 | 1.32 | 1.72E7 | 3.57E-4 |
| Ru-103 | 39.26d | 3.23E4 | 2.65 | 1.20E6 | 7.17E-4 |
| Ru-105 | 4.44h | 6.73E6 | 1.93 | 2.49E8 | 5.22E-4 |
| Ru-106 | 1.02y | 3.31E3 | N/A | 1.22E5 | N/A |
| S-35 | 87.51d | 4.27E4 | N/A | 1.58E6 | N/A |
| Sb-122 | 2.7238d | 3.93E5 | 2.991 | 1.46E7 | 8.10E-4 |
| Sb-124 | 60.2d | 1.75E4 | 9.62 | 6.48E5 | 2.60E-3 |
| Sb-125 | 1007.4d | 1.04E3 | 2.57 | 3.84E4 | 6.96E-4 |
| Sb-126 | 12.46d | 8.33E4 | 11.5 | 3.08E6 | 3.11E-3 |
| Sc-44 | 3.927h | 1.82E7 | 0.579 | 6.72E8 | 1.57E-4 |
| Sc-46 | 83.81d | 3.39E4 | 10.9 | 1.25E6 | 2.95E-3 |
| Sc-47 | 3.349d | 8.30E5 | 0.56 | 3.07E7 | 1.51E-4 |
| Sc-48 | 43.7h | 1.49E6 | 21 | 5.51E7 | 5.68E-3 |
| Se-75 | 119.78d | 1.45E4 | 9.53 | 5.37E5 | 2.58E-3 |
| Se-79 | 6.50E5y | 6.98E-3 | N/A | 0.258 | N/A |
| Si-32 | 132y | 84.77 | N/A | 3.14E3 | N/A |
| Sm-146 | 1.031E8y | 2.38E-5 | N/A | 8.80E-4 | N/A |
| Sm-147 | 1.06E11y | 2.30E-8 | N/A | 8.50E-7 | N/A |
| Sm-148 | 7.00E15y | 3.46E-13 | N/A | 1.28E-11 | N/A |

| | Half-Life | Ci/g | Rem/hr / Ci | Sv/hr / GBq |
|---------|------------------|-------------|--------------------|--------------------|
| | | | @ 30 cm | @ 30cm |
| Sm-153 | 46.27h | 4.43E5 | 0.175 | 1.64E7 |
| Sn-121 | 27.06h | 9.58E5 | N/A | 3.54E7 |
| Sn-125 | 9.64d | 1.09E5 | 0.33 | 4.01E6 |
| Sr-85 | 64.84d | 2.37E4 | 3.06 | 8.78E5 |
| Sr-87m | 2.803h | 1.32E7 | 1.92 | 4.87E8 |
| Sr-89 | 50.52d | 2.90E4 | 5.29E-3 | 1.07E6 |
| Sr-90 | 29.1y | 137.0 | N/A | 5.07E3 |
| Sr-91 | 9.63h | 3.58E6 | 0.635 | 1.32E8 |
| Sr-92 | 2.71h | 1.26E7 | 7.8942 | 4.65E8 |
| Tb-160 | 72.3d | 1.13E4 | 0.635 | 4.18E5 |
| Tc-99 | 2.13E5y | 0.017 | N/A | 0.629 |
| Tc-99m | 6.01h | 5.27E6 | 0.896 | 1.95E8 |
| Tc-101 | 14.2m | 1.31E8 | 1.71 | 4.85E9 |
| Te-123m | 119.7d | 8.88E3 | 1.365 | 3.28E5 |
| Te-127 | 9.35h | 2.64E6 | 0.0335 | 9.78E7 |
| Te-129 | 69.6m | 2.10E7 | 0.5717 | 7.76E8 |
| Te-129m | 33.6d | 3.02E4 | 0.137 | 1.12E6 |
| Te-131 | 25m | 5.75E7 | 1.57 | 2.13E9 |
| Te-131m | 30h | 7.98E5 | 2.18 | 2.95E7 |
| Te-132 | 3.204d | 3.09E5 | 2.124 | 1.14E7 |
| Te-133 | 12.5m | 1.13E8 | 2.32 | 4.19E9 |
| Te-133m | 55.4m | 2.55E7 | 3.11 | 9.45E8 |
| Te-134 | 41.8m | 3.36E7 | 1.77 | 1.24E9 |
| Te-135 | 19s | 4.40E9 | 0.195 | 1.63E11 |
| Th-227 | 18.72d | 3.07E4 | 0.39 | 1.14E6 |
| Th-228 | 1.913y | 820.0 | 0.014 | 3.03E4 |
| Th-229 | 7300y | 0.214 | 0.145 | 7.92 |
| Th-230 | 7.54E4y | 0.021 | 2.07E-3 | 0.762 |
| Th-231 | 25.55h | 5.32E5 | 0.0480 | 1.97E7 |
| Th-232 | 1.40E10y | 1.10E-7 | 7.62E-4 | 4.07E-6 |
| Th-234 | 24.10d | 2.32E4 | 0.0356 | 8.58E5 |

| | Half-Life | Ci/g | Rem/hr / Ci | | Sv/hr / GBq |
|---------|------------------|-------------|--------------------|--------------|--------------------|
| | | | @ 30 cm | GBq/g | @ 30cm |
| TI-201 | 72.912h | 2.14E5 | 0.122 | 7.91E6 | 3.30E-5 |
| TI-204 | 3.78y | 464.0 | 0.0124 | 1.72E4 | 3.35E-6 |
| TI-206 | 4.20m | 2.17E8 | N/A | 8.03E9 | N/A |
| TI-208 | 3.053m | 2.96E8 | 18.89 | 1.10E10 | 5.11E-3 |
| TI-209 | 2.161m | 4.16E8 | 4.17 | 1.54E10 | 1.13E-3 |
| TI-210 | 1.30m | 6.88E8 | 7.82 | 2.55E10 | 2.11E-3 |
| U-230 | 20.8d | 2.73E4 | 2.00E-3 | 1.01E6 | 5.41E-7 |
| U-232 | 70y | 22.0 | 0.0731 | 814 | 1.98E-5 |
| U-233 | 1.592E5y | 9.65E-3 | N/A | 0.357 | N/A |
| U-234 | 2.46E5y | 6.22E-3 | N/A | 0.230 | N/A |
| U-235 | 7.04E8y | 2.16E-6 | 0.755 | 7.99E-5 | 2.04E-4 |
| U-235m | 25.0m | 3.20E7 | N/A | 1.18E9 | N/A |
| U-236 | 2.342E7y | 6.47E-5 | 1.10E-4 | 2.40E-3 | 2.98E-8 |
| U-237 | 6.75d | 8.16E4 | 0.561 | 3.02E6 | 1.52E-4 |
| U-238 | 4.47E9y | 3.36E-7 | N/A | 1.24E-5 | N/A |
| V-48 | 15.98d | 1.70E5 | 15.6 | 6.29E6 | 4.22E-3 |
| V-49 | 330d | 8.09E3 | N/A | 2.99E5 | N/A |
| W-187 | 23.72d | 7.07E5 | 2.82 | 2.62E7 | 7.63E-4 |
| Xe-131m | 11.84d | 8.69E4 | 0.5664 | 3.22E6 | 1.53E-4 |
| Xe-133 | 5.243d | 1.87E5 | 0.6248 | 6.93E6 | 1.69E-4 |
| Xe-133m | 2.19d | 4.49E5 | 0.7027 | 1.66E7 | 1.90E-4 |
| Xe-135 | 9.14h | 2.54E6 | 1.6178 | 9.41E7 | 4.38E-4 |
| Xe-135m | 15.29m | 9.12E7 | 2.9736 | 3.37E9 | 8.05E-4 |
| Xe-138 | 14.08m | 9.69E7 | 1.36 | 3.58E9 | 3.68E-4 |
| Y-88 | 106.65d | 1.39E4 | 14.83 | 5.15E5 | 4.01E-3 |
| Y-90 | 64.1h | 5.43E5 | N/A | 2.01E7 | N/A |
| Y-92 | 3.54h | 9.63E6 | 0.126 | 3.56E8 | 3.41E-5 |
| Y-93 | 10.18h | 3.31E6 | 0.11 | 1.23E8 | 2.98E-5 |
| Yb-169 | 32.026d | 2.41E4 | 1.219 | 8.93E5 | 3.30E-4 |
| Zn-65 | 243.8d | 8.24E3 | 3.575 | 3.05E5 | 9.68E-4 |
| Zr-89 | 78.41h | 4.50E5 | 5.65 | 1.66E7 | 1.53E-3 |

| | Half-Life | Ci/g | Rem/hr / Ci @ 30 cm | GBq/g | Sv/hr / GBq @ 30cm |
|-------|------------------|-------------|--------------------------------|--------------|-------------------------------|
| Zr-93 | 1.53E6y | 2.52E-3 | N/A | 0.0931 | N/A |
| Zr-95 | 64.02d | 2.15E4 | 5.16 | 7.96E5 | 1.39E-3 |
| Zr-97 | 16.91h | 1.91E6 | 0.236 | 7.08E7 | 6.39E-5 |

The exposure rate from these radionuclides do not include their short-lived progeny. Spontaneous fission, isotopic mixtures, impurities in mixtures, and shielding (including self shielding) should also be taken into account when estimating exposure rate.

**Gamma exposure at 30 cm vs Particle Size
in microns for commonly encountered radionuclides**

| | mRem/hr | | | mSv/hr | | |
|---------|---------|--------|--------|---------|--------|--------|
| | 1μ | 10μ | 100μ | 1μ | 10μ | 100μ |
| Be-7 | 1.3E-4 | 1.3E-1 | 1.3E2 | 1.3E-6 | 1.3E-3 | 1.3 |
| Na-22 | 4.7E-5 | 4.7E-2 | 4.7E1 | 4.7E-7 | 4.7E-4 | 0.47 |
| Na-24 | 9.5E-2 | 9.5E1 | 9.5E4 | 9.5E-4 | 0.95 | 9.5E2 |
| Al-26 | 4.5E-10 | 4.5E-7 | 4.5E-4 | 4.5E-12 | 4.5E-9 | 4.5E-7 |
| Mg-28 | 4.8E-2 | 4.8E1 | 4.8E4 | 4.8E-4 | 0.48 | 4.8E2 |
| Sc-46 | 6.9E-4 | 6.9E-1 | 6.9E2 | 6.9E-6 | 6.9E-4 | 6.9 |
| V-48 | 1E-2 | 1E1 | 1E4 | 1E-4 | 0.10 | 1E2 |
| Cr-51 | 9E-5 | 9E-2 | 9E1 | 9E-7 | 9E-4 | 0.9 |
| Mn-52 | 3.8E-2 | 3.8E1 | 3.8E4 | 3.8E-4 | 0.38 | 3.8E2 |
| Mn-54 | 1.7E-4 | 1.7E-1 | 1.7E2 | 1.7E-6 | 1.7E-3 | 1.7 |
| Mn-56 | 8.3E-1 | 8.3E2 | 8.3E5 | 8.3E-3 | 8.3 | 8.3E3 |
| Co-56 | 2.9E-3 | 2.9 | 2.9E3 | 2.9E-5 | 2.9E-2 | 29 |
| Co-57 | 6.6E-5 | 6.6E-2 | 6.6E1 | 6.6E-7 | 6.6E-4 | 0.66 |
| Co-58 | 1E-3 | 1 | 1E3 | 1E-5 | 1E-2 | 10 |
| Fe-59 | 1.5E-3 | 1.5 | 1.5E3 | 1.5E-5 | 1.5E-2 | 15 |
| Co-60 | 8E-5 | 8E-2 | 8E1 | 8E-7 | 8E-4 | 0.8 |
| Zn-65 | 1.1E-4 | 1.1E-1 | 1.1E2 | 1.1E-6 | 1.1E-3 | 1.1 |
| Se-75 | 3.5E-4 | 3.5E-1 | 3.5E2 | 3.5E-6 | 3.5E-3 | 3.5 |
| Y-88 | 6.3E-4 | 6.3E-1 | 6.3E2 | 6.3E-6 | 6.3E-3 | 6.3 |
| Sr/Y-90 | N/A | N/A | N/A | N/A | N/A | N/A |
| Zr-95 | 3.8E-4 | 3.8E-1 | 3.8E2 | 3.8E-6 | 3.8E-3 | 3.8 |
| Mo-99 | 3.2E-3 | 3.2 | 3.2E3 | 3.2E-5 | 3.2E-2 | 32 |
| Cd-109 | 2.4E-5 | 2.4E-2 | 2.4E1 | 2.4E-7 | 2.4E-4 | 0.24 |
| Cs-137 | 3.6E-7 | 3.6E-4 | 3.6E-1 | 3.6E-9 | 3.6E-6 | 3.6E-3 |
| Ba-140 | 2.4E-4 | 2.4E-1 | 2.4E2 | 2.4E-6 | 2.4E-3 | 2.4 |
| W-187 | 1.1E-3 | 1.1 | 1.1E3 | 1.1E-5 | 1.1E-2 | 11 |
| Os-191 | 3.9E-4 | 3.9E-1 | 3.9E2 | 3.9E-6 | 3.9E-3 | 3.9 |
| Ir-192 | 7.1E-4 | 7.1E-1 | 7.1E2 | 7.1E-6 | 7.1E-3 | 7.1 |
| Au-198 | 8E-3 | 8 | 8E3 | 8E-5 | 8E-2 | 80 |

| | mRem/hr | | | mSv/hr | | |
|--------|---------|---------|--------|---------|---------|---------|
| | 1μ | 10μ | 100μ | 1μ | 10μ | 100μ |
| Ra-226 | 3.5E-10 | 3.5E-7 | 3.5E-4 | 3.5E-12 | 3.5E-9 | 3.5E-6 |
| U-234 | 5.4E-11 | 5.4E-8 | 5.4E-5 | 5.4E-13 | 5.4E-10 | 5.4E-7 |
| U-235 | 8.1E-14 | 8.1E-11 | 8.1E-8 | 8.1E-16 | 8.1E-13 | 8.1E-10 |
| Np-237 | 3.9E-11 | 3.9E-8 | 3.9E-5 | 3.9E-13 | 3.9E-10 | 3.9E-7 |
| Pu-238 | 1.6E-7 | 1.6E-4 | 1.6E-1 | 1.6E-9 | 1.6E-6 | 1.6E-3 |
| Pu-239 | 2.2E-10 | 2.2E-7 | 2.2E-4 | 2.2E-12 | 2.2E-9 | 2.2E-6 |
| Pu-240 | 2E-9 | 2E-6 | 2E-3 | 2E-11 | 2E-8 | 2E-5 |
| Am-241 | 1.3E-7 | 1.3E-4 | 1.3E-1 | 1.3E-9 | 1.3E-6 | 1.3E-3 |

1000 μ = 1 mm (millimeter) = 0.03937 inches

100 μ is easily discernible with the naked eye

50 μ is not easily discernible with the naked eye

< 10 μ is typical size for airborne particles

**Activity in DPM vs Particle Size in microns
for oxide form of various isotopes**

| | 0.5μ | 1μ | 5μ | 10μ | 50μ |
|--------|-------------|-----------|-----------|------------|------------|
| U-234 | 8.7E-3 | 0.07 | 9 | 69.7 | 8700 |
| U-235 | 3.0E-6 | 2.4E-5 | 3E-3 | 0.02 | 3 |
| U-238 | 4.7E-7 | 3.8E-6 | 5E-4 | 3.8E-3 | 0.47 |
| Np-237 | 1.0E-3 | 8.0E-3 | 1.0 | 8 | 1.0E3 |
| Pu-238 | 25 | 201 | 2.5E4 | 2E5 | 2.5E7 |
| Pu-239 | 0.09 | 0.73 | 91 | 730 | 9.1E4 |
| Pu-240 | 0.33 | 2.7 | 333 | 2.67E3 | 3.3E5 |
| Pu-241 | 151 | 1.21E3 | 1.5E5 | 1.2E6 | 1.5E8 |
| Am-241 | 5.1 | 41.1 | 5.14E3 | 4.1E4 | 5.14E6 |

Calculating Activity vs Particle Size

1. Volume of the particle is $V = 1/6\pi d^3$.
2. Use the density of the isotope listed in this reference.
3. Mass of the particle is $M = V \times \text{density}$.
4. Activity of the particle is $A = M \times \text{specific activity}$.

Correct the activity of the particle for the oxide form if you need that; the molecular weight of Pu-238 is 238, the activity of the dioxide form must be reduced by the ratio of the molecular weight of the dioxide form to the molecular weight of Pu-238. Multiply the calculated activity by 238/270 to get the activity of the dioxide form.

For particles larger than about 1μ the aerodynamic diameter is approximately equal to the physical diameter times the square root of the density. The 10μ diameter particle in our example would have an equivalent aerodynamic diameter of 34μ (10μ x the square root of 11.46). This must be taken into account in air sampling/monitoring situations.

RADIATION BIOLOGY

Maximum survivable dose: 1000 rem (10 Sv)

Cancer mortality rate ~ 900 excess deaths per 100,000 persons at 0.1 Sv (10 rem)

Radiation Dose Risk

| | |
|--|------------------------------------|
| Report | Additional Cancer Deaths |
| BEIR III 1980 (also Reg Guide 8.29) | 3 in 10,000 per 1 rem (10 mSv) |
| BEIR V 1990 | 800 in 100,000 per 10 rad (0.1 Gy) |

Hiroshima Survivors Incidence of Cancer

4,000 Hiroshima survivors who received doses greater than 50 rem showed an extra 300 incidences of cancer.

COMPOSITION OF THE HUMAN BODY

| | | | | | |
|----|--------|----|-----------|----|----------|
| O | 65 % | Rb | 0.00046 % | I | 1.6E-5 % |
| C | 18 | Sr | 0.00046 | Au | 1.4E-5 |
| H | 10 | Br | 0.00029 | Ni | 1.4E-5 |
| N | 3 | Pb | 0.00017 | Mo | 1.3E-5 |
| Ca | 1.5 | Nb | 0.00016 | Ti | 1.3E-5 |
| P | 1.0 | Cu | 0.00010 | Te | 1.2E-5 |
| S | 0.25 | Al | 0.000087 | Sb | 1.1E-5 |
| K | 0.20 | Cd | 0.000072 | Li | 3.11E-6 |
| Cl | 0.15 | B | 0.000069 | Cr | 2.4E-6 |
| Na | 0.15 | Ba | 0.000031 | Cs | 2.1E-6 |
| Mg | 0.05 | As | 0.000026 | Co | 2.1E-6 |
| Fe | 0.006 | V | 0.000026 | Ag | 1.0E-6 |
| F | 0.0037 | Sn | 0.000024 | U | 1.3E-7 |
| Zn | 0.0032 | Hg | 0.000019 | Be | 5E-8 |
| Si | 0.0020 | Se | 0.000019 | Ra | 1E-13 |
| Zr | 0.0006 | Mn | 0.00001 | | |

DOSIMETRY

1 Bq = 1 dps = 2.7 E-11 Ci
1 Gy = 1 joule / kg = 100 rads

$$H_T (\text{Sv}) = D(\text{Gy}) \times Q (\text{Sv} / \text{Gy})$$

Quality Factors (Q) values:

x-rays, beta, gamma = 1
neutrons: thermal = 2
 fast = 10
alpha = 20

DOSE EQUIVALENT CALCULATIONS

1 Roentgen = 2.58E-4C / kg or 1 esu / cm³
 = 87 ergs / g or 2.082 E9 ip / cm³
 = 7.02 E4 MeV / cm³ in air @ STP
or = 98 ergs / g in tissue

1 R/hr ~ 1 E-13 Amperes / cm³

1 rad = 100 ergs / g in any absorber

ρ_{air} = 0.001293 g / cm³

W_{air} = 33.7 eV

1 Ampere = 1 Coulomb / sec

STP_{air} = 760mm Hg @ 0⁰C or 14.7lb / in² @ 32⁰ F

INTERNAL DOSIMETRY

Calculating CDE and CEDE ICRP 26/30

CDE = $I / nALI \times 50 \text{ rem (0.5 Sv)}$ nALI is the non-stochastic ALI

CDE = 50 yr committed dose equivalent to irradiated tissue
I = Intake

nALI = non-stochastic ALI = $50 \text{ rem (0.5 Sv)} / h_{\max}$

h_{\max} = greatest dose equivalent found in the exposure-to-dose conversion tables

CEDE = $I / sALI \times 5 \text{ rem (50 mSv)}$ sALI is the stochastic ALI

CEDE = 50 yr committed effective dose equivalent

OR CEDE = $\sum_{i=1}^n W_T$

CEDE = 50 yr committed effective dose equivalent to individual tissue

W_T = tissue weighting factor

Effective Dose Equivalent EDE = $H_{\Sigma} = \sum W_T H_T$

D.E. rate (Sv / hr) = $0.15 A(\text{TBq})E / r^2$

Calculating DAC and DAC-hours

DAC = ALI / 2000 hr at 1.2 E6 ml / hr

1 DAC-h = 2.5 mrem (25 μSv) CEDE if based on sALI OR
25 mrem (0.25 mSv) ref ICRP 26 CDE to an organ or tissue if based on nALI

DAC Fraction = $\sum_i (\text{concentration} / \text{DAC}) / \text{PF}$

DAC fraction x time (hours) = DAC-hours

INTERNAL DOSIMETRY

Intake I(Bq) = $A_t(\text{Bq}) / \text{IRF}_t$

Body burden q = $q_0 e^{-\lambda_{\text{eff}} t}$

CEDE or H_{50} = $50 \text{ mSv (5 rem)} \times I / \text{ALI}$

TEDE = CEDE + Deep Dose Equivalent

INTERNAL DOSIMETRY

Effective Half-Life

$$t_{\text{eff}} = t_r \times t_b / (t_r + t_b)$$

where; t_r = radioactive half-life

t_b = biological half-life

Effective Removal Constant

$$\lambda_{\text{eff}} = \lambda_r + \lambda_b$$

where; λ_r = decay constant = $-0.693 / t_{1/2}$

λ_b = biological removal constant $-0.693 / t_b$

Calculating Internal Dose (ICRP 30)

$$H_{50} (\text{T-S}) = (1.6E-10)U_S \text{ SEE(T-S)}$$

H_{50} = 50 year dose equivalent commitment in sieverts
where SEE is the Specific Effective Energy modified by a quality factor for radiation absorbed in the target organ (T) for each transformation in the source organ (S) expressed in MeV/g.

$$\text{SEE} = \sum Y \cdot E \cdot AF \cdot Q / M_T$$

where:

Y = yield of radiations per transformation

E = average energy of the radiation

AF = absorbed fraction of energy absorbed in the target organ (T) per emission of radiation in the source organ (S)

Q = quality factor

M_T = mass of the target organ

U_S = number of nuclear transformations in the source organ (S) during the time interval for which the dose is to be calculated

EQUIVALENT DOSE, EFFECTIVE DOSE, and COMMITTED EFFECTIVE DOSE

ICRP 60 Equivalent Dose

$H_T = \sum_R W_R D_{T,R}$
 H_T = equivalent dose in tissue T
 W_R = radiation weighting factor
 $D_{T,R}$ = absorbed dose averaged over tissue T due to radiation R

ICRP 60 Effective Dose

$E = \sum_T W_T H_T$
 E = effective dose to the individual
 W_T = tissue weighting factor
 H_T = equivalent dose in tissue(s) T

ICRP 60 Committed Effective Dose

$E(50) = \frac{\sum_{T=1}^{T=j} W_T H_T(50) + (W_{\text{remainder}} \sum_{T=K}^{T=1} M_T H_T(50))}{\sum_{T=K}^{T=1} M_T}$
 $E(50)$ = committed effective dose
 W_T = tissue weighting factor for tissues & organs T_i to T_j
 M_T = mass of the remainder tissues T_K to T_1
 $W_{\text{remainder}}$ = 0.05 (the W_T assigned to the remainder tissues)

ICRP 23 REFERENCE MAN

Daily Water Intake = 2.2 liters / day
Breathing Rate = 2 E4 ml / min
Skin surface area = 18,000 cm²

There are approximately 10^{13} cells in the human body.

There are 140 g of potassium in reference man, 125 nCi (4.625 kBq) is K⁴⁰ which results in 0.25 mrem/wk or 13 mrem/yr (2.5 μ Sv/wk or 0.13 mSv/yr) to the whole body.

RADIATION WEIGHTING FACTORS¹ (ICRP 60)

| Type and Energy Range ² | Radiation Weighting Factor, W_R |
|---|-----------------------------------|
| Photons, all energies | 1 |
| Electrons and muons, all energies ³ | 1 |
| Neutrons, <10 keV | 5 |
| 10 keV to 100 keV | 10 |
| 100 keV to 2 MeV | 20 |
| 2 MeV to 20 MeV | 10 |
| > 20 MeV | 5 |
| Protons, other than recoil protons, energy > 2MeV | 5 |
| Alpha particles, fission fragments, heavy nuclei | 20 |

¹All values relate to the radiation incident on the body or, for internal sources, emitted from the source.

²The choice of values for other radiation is discussed in Annex A of Publication 60.

³Excluding Auger electrons emitted from nuclei bound to DNA

ICRP 60 Tissue Weighting Factors

| Tissue or organ | Tissue weighting factor, W_T |
|-------------------|--------------------------------|
| Gonads | 0.20 |
| Bone marrow (red) | 0.12 |
| Colon | 0.12 |
| Lung | 0.12 |
| Stomach | 0.12 |
| Bladder | 0.05 |
| Breast | 0.05 |
| Liver | 0.05 |
| Oesophagus | 0.05 |
| Thyroid | 0.05 |
| Skin | 0.01 |
| Bone surface | 0.01 |
| Remainder | 0.05 |

CALCULATING TODE AND TEDE

| | | |
|------|---|--|
| TEDE | = | DDE + CEDE |
| TODE | = | DDE + CDE |
| TEDE | = | total effective dose equivalent |
| TODE | = | total organ dose equivalent |
| DDE | = | deep dose equivalent |
| CDE | = | 50 year committed dose equivalent to a tissue or organ |
| CEDE | = | 50 year committed effective dose equivalent |

DOSE EQUIVALENT LIMITS & POSTING REQUIREMENTS (10CFR20 & 10CFR835)

| Dose Equivalent | Annual Limit |
|----------------------------|----------------|
| TEDE | 5 rem 50 mSv |
| TODE | 50 rem 0.5 Sv |
| LDE (Lens Dose Equivalent) | 15 rem 0.15 Sv |
| SDE, WB | 50 rem 0.5 Sv |
| SDE, ME | 50 rem 0.5 Sv |
| TEDE (general public) | 0.1 rem 1 mSv |

DOSE EQUIVALENT MEASUREMENT

Abbreviations from USNRC Reg. Guide 8.7

| | Measurement Depth for External Sources (cm) | Density Thickness (mg / cm ²) |
|----------------------|---|---|
| TEDE | 1 | 1000 |
| TODE | 1 | 1000 |
| LDE | 0.3 | 300 |
| SDE, WB ¹ | 0.007 | 7 |
| SDE, ME ² | 0.007 | 7 |

¹SDE, WB is the shallow dose equivalent to the skin of the whole body

²SDE, ME the shallow dose equivalent to a major extremity.

RADIATION INTERACTIONS

Charged Particles

Ionization, Excitation, *Bremsstrahlung* (β^-), Annihilation (β^+)

Neutrons

Scattering ($E > 0.025 \text{ eV}$)

Elastic (energy and momentum are conserved)

Inelastic (photon emitted)

Absorption ($E < 0.025 \text{ eV}$)

Radiative Capture (η, γ)

Particle Emission (η, α) (η, p) (η, η)

Fission (η, f)

Gamma or X-ray photons

Photoelectric Effect (generally $\leq 1 \text{ MeV}$)

Compton Scattering (generally 200 keV - 5 MeV)

Pair Production (minimum 1.022 MeV)

Scattered Photon

$$T' = T / [1 + T(1 - \cos \Theta) / m_0 c_2] \quad \text{where } c_2 = 931.5 \text{ MeV / amu}$$

Bremsstrahlung

emitted energy is $\sim 1/3$ of the electron energy

Photon Attenuation: $I_x = I_0 e^{-\mu x}$

Interaction Probability per gram:

Photoelectric $\sim Z^4 / E^3$

Compton independent of Z

Pair Production $\sim Z^1$

$$\mu_{\text{Total}} = \mu_{\text{pe}} + \mu_{\text{cs}} + \mu_{\text{pp}}$$

$$W_{\text{Air}} = 33.9 \text{ eV per ion pair}$$

$$\text{Specific Ionization} = S/W \text{ (i.p. / cm)}$$

SHIELDING MATERIALS

| | |
|------------------------|---|
| α | N/A |
| β^- | low Z, such as plastic or aluminum |
| γ | high Z, such as tungsten |
| mixed β^-/γ | low Z, then high Z |
| neutron | hydrogenous material to thermalize (such as polyethylene) then neutron absorber (such as Cd, B, Li, Hf), then high Z to absorb "capture gammas" |

Photon Half-Value Layers in CM

| MeV | 0.10 | 0.60 | 1.00 | 2.00 | 6.00 | 15.00 |
|----------|-------|------|------|------|------|-------|
| U | 0.005 | 0.25 | 0.48 | 0.78 | 0.80 | 0.62 |
| W | 0.008 | 0.35 | 0.58 | 0.82 | 0.85 | 0.67 |
| Pb | 0.012 | 0.52 | 0.90 | 1.35 | 1.39 | 1.08 |
| Sn | 0.06 | 1.20 | 1.38 | 1.80 | 2.65 | 2.20 |
| Cu | 0.18 | 1.01 | 1.70 | 1.65 | 2.49 | 2.38 |
| Fe | 0.25 | 1.15 | 1.32 | 1.55 | 2.88 | 2.85 |
| Al | 1.12 | 3.30 | 4.45 | 5.90 | 9.67 | 11.7 |
| Concrete | 1.8 | 3.8 | 4.6 | 6.2 | 11.2 | 10.4 |
| Water | 4.20 | 7.80 | 9.60 | 14.2 | 25.0 | 35.7 |

This table applies to a thin shield and no provision is made for buildup factor. Always perform a radiation measurement to confirm adequacy of shield.

Tenth-value Thickness

Simply multiply the half-value thickness by the square root of 10 (3.162) to get the tenth-value thickness.

Example: A half-value thickness of concrete for Cs-137 gamma radiation is 3.8 cm.

The tenth-value thickness is $3.8 \text{ cm} \times 3.162 = 12 \text{ cm}$.

Neutron and Gamma Shielding

SIMPLIFIED SHIELD THICKNESS CALCULATION

perform radiation measurements to verify these calculations

I = shielded exposure rate

I_0 = unshielded exposure rate

n = number of shielding layers (tenth or half)

I = $I_0 \times 0.1^n$ for tenth value thickness

I = $I_0 \times 0.5^n$ for half value thickness

Incorporating Photon Buildup Factors

I = $I_0 \times B \times 0.5^n$

I = $I_0 \times B \times e^{-\mu x}$

μ is the linear attenuation coefficient in - cm

x is the shield thickness in cm

B is the buildup factor taken from tables, obtained by measurements, or calculations such as MCNP.

Radiation Streaming

Consider the potential for radiation streaming thru gaps in the shielding. Design the shielding to minimize gaps and perform a comprehensive survey after the shielding is in place.

Stay-Time Calculation

Stay-time calculations are typically used to determine how long an individual can remain in an area with elevated radiation fields until they reach some pre-determined dose limit. The principles can also be applied to airborne areas.

Stay-time = Allowable exposure/exposure rate

example; allowable exposure is 100 mR
exposure rate is 25 mR/hr

Stay-time = $100 \text{ mR} / 25 \text{ mR/hr} = 4 \text{ hours}$

Beta Dose Rates

| MeV | rad/h per mCi | | | Gy/h per MBq | | |
|------|---------------|-------|-------|--------------|-------|-------|
| | 1 cm | 10 cm | 30 cm | 1 cm | 10 cm | 30 cm |
| 0.15 | 1,200 | 1.7 | 0 | 444 | 0.6 | 0 |
| 0.25 | 1,000 | 2.2 | 0.1 | 370 | 0.81 | 0.037 |
| 0.30 | 900 | 3.6 | 0.1 | 333 | 1.33 | 0.037 |
| 0.50 | 750 | 5.2 | 0.4 | 278 | 1.92 | 0.148 |
| 0.75 | 650 | 5.0 | 0.5 | 241 | 1.85 | 0.185 |
| 1.0 | 550 | 4.6 | 0.4 | 204 | 1.70 | 0.148 |
| 1.25 | 450 | 4.3 | 0.4 | 167 | 1.59 | 0.148 |
| 1.50 | 400 | 4.0 | 0.4 | 148 | 1.48 | 0.148 |
| 1.75 | 350 | 3.4 | 0.4 | 130 | 1.26 | 0.148 |
| 2.00 | 340 | 3.6 | 0.4 | 126 | 1.33 | 0.148 |
| 2.25 | 320 | 3.3 | 0.4 | 118 | 1.22 | 0.148 |

Beta dose should be treated as a “shallow” dose and should not be summed with “deep” doses. This chart should also be used to determine beta⁺ doses from positron emitters.

Half-value Thickness vs Beta Energy

| Isotope | Emax (MeV) | Half-Value Thickness mg / cm ² |
|--------------------------------------|---------------|---|
| C-14 | 0.156 | 2 |
| Tc-99 | 0.292 | 7.5 |
| Cl-36 | 0.714 | 15 |
| Sr/Y-90 | 0.546 / 2.284 | 150 |
| U-238 Betas from short lived progeny | | |
| | 0.191 / 2.281 | 130 |
| P-32 | 1.710 | 150 |

Estimate the half-value thickness for a beta emitter.

$$\text{mg/cm}^2 = 50 \times E^2$$

where E is Emax in MeV for the beta emitter

This equation tends to underestimate the half-value thickness for low energy betas and overestimate the half-value thickness for high energy betas.

Positron Emitters Beta⁺ Energy and % Abundance

| | Half-life | MeV (%) |
|-------|-----------|------------------------------|
| C-11 | 20.3m | 0.960 (99.8%) |
| N-13 | 9.97m | 1.199 (99.8%) |
| O-15 | 122s | 1.732 (99.9%) |
| F-18 | 1.83h | 0.634 (96.7%) |
| Na-22 | 2.605y | 0.546 (89.8%) |
| Al-26 | 7.3E5y | 3.210 (100%) |
| V-48 | 15.98d | 0.697 (50.1%) |
| Mn-52 | 5.591d | 2.633 (94.9%) |
| Co-56 | 77.3d | 1.458 (19.0%) |
| Ni-57 | 35.6h | 0.737 (7.0%), 0.865 (35.3%) |
| Co-58 | 70.88d | 0.475 (14.9%) |
| Cu-62 | 9.74m | 2.926 (97.2%) |
| Zn-65 | 243.8d | 0.330 (1.4%) |
| Ga-68 | 67.7m | 0.822 (1.2%), 1.899 (89.1%) |
| As-74 | 17.8d | 0.945 (26.1%), 1.540 (3.0%) |
| Rb-82 | 1.26m | 2.601 (13.1%), 3.378 (81.8%) |

Several of the positron emitters are useful in PET studies. That usefulness is somewhat offset by the cost of producing the radionuclides and the added complexity of radiation protection. For all of the positron emitters the energy of the Beta+ must be considered. Refer to the table of Beta Dose Rates for estimates of beta⁺ radiation exposure. Also, consider the annihilation photons when the positron comes into contact with a beta-, annihilating their masses and producing two 511 KeV photons. These photons present an external radiation hazard. For the patient undergoing a PET scan the combination of the positron energy and the photon energy must be considered.

Combining Radiation Types to Determine Total Dose

An individual radionuclide may have several different types of emissions. Those different types of emissions and the shortlived progeny of the individual radionuclide must be considered when determining a total dose.

Particulate radiation should be treated as a “shallow” dose while photons and neutrons should be treated as a “deep” dose and these two types of doses should not be summed. This example with sodium-22 will clarify this concept.

Na-22 2.605y Beta⁺ 0.546 MeV (89.8% Abundance)
1 mCi Gamma 1.275 MeV (99.9% Abundance)

From the table of Beta Dose Rates we find 320 rad/hr at 1 cm and 0.4 rad/hr at 30 cm. The near contact dose rate is much higher than the dose rate at 30 cm.

Using 6CEN for the gamma dose rate we find;

$$\begin{aligned} 6\text{CEN} &= 6 \times 1 \text{ mCi} \times 1.275 \text{ MeV} \times 0.999 \\ &= 7.64 \text{ mRem/hr at 1 foot } (\sim 30 \text{ cm}). \end{aligned}$$

We can also use 6CEN for the annihilation photons from the positron.

$$\begin{aligned} 6\text{CEN} &= 6 \times 1 \text{ mCi} \times 0.511 \text{ MeV} \times 2 \times 0.898 \\ &= 5.51 \text{ mRem/hr at 1 foot } (\sim 30 \text{ cm}). \end{aligned}$$

The “shallow” dose from the positron at 30 cm is 400 mrad/hr and the “deep” dose from the gamma and photon radiation is 7.64 mRem/hr + 5.51 mRem/hr = 13.15 mRem/hr.

Shallow Dose Correction Factor

In accordance with 10CFR20 and 10CFR835 deep dose equivalent shall be used for posting of radiation areas. Shallow dose equivalent shall be reported separate from deep dose equivalent. Deep dose equivalent is the sum of the gamma and neutron deep dose equivalents. Shallow dose includes low-energy photons and charged particles such as betas, positrons, and protons. Alpha particles are not included in shallow dose.

The following applies to vented air ionization chambers with a window density thickness of 7 mg/cm^2 and a moveable shield with a density thickness of $1,000 \text{ mg/cm}^2$.

Determining the need to report a shallow dose;
If the Open Shield Reading divided by the Closed Shield Reading is equal to or greater than 1.2, then perform a shallow dose survey.

Calculate the shallow dose rate using this equation;
 $(\text{Open Shield Reading} - \text{Closed Shield Reading}) \times \text{CF}$
Obtain the **CF** (Correction Factor) from experimental or published data for the specific detector and radiation source(s).

Typical correction factors for betas range between 2 and 5 (multipliers).

Typical correction factors for low energy photons range between 0.1 and 1 (multipliers).

Low energy photons that penetrate the closed shield of the ion chamber and produce a response in the instrument are part of the “deep” dose.

NEUTRON SHIELD THICKNESS

$$I = I_0 e^{-\sigma N x}$$

where; I = final neutron flux rate

I_0 = initial neutron flux rate

σ = shield cross section in square centimeters

N = number of atoms per cm^3 in the shield

x = shield thickness in centimeters

example:

A dosimetry phantom is designed to simulate the composition of the human body. Ten % by weight is hydrogen. Assume a density of 1 and a shield cross section of hydrogen of 0.1 barns. A barn is $1\text{E}-24 \text{ cm}^2$. N , the number of atoms per cm^3 , is 10% of Avogadro's number, so N equals $6\text{E}22$ hydrogen atoms per cm^3 . Assume the phantom thickness is 30 cm.

$$I^0 = 5,000 \text{ n/cm}^2 / \text{s}$$

$$\sigma = 1\text{E}-25 \text{ cm}^2 (0.1 \text{ barns})$$

$$N = 6\text{E}22 \text{ atoms per } \text{cm}^3$$

$$x = 30 \text{ centimeters thick}$$

$$-\sigma N x = 1\text{E}-25 \text{ times } 6\text{E}22 \text{ times } 30 = -0.18$$

$$I = I_0 e^{-\sigma N x}$$

$$I = 5,000 \text{ n/cm}^2 / \text{s } e^{-0.18}$$

$$I = 5,000 \text{ n/cm}^2 / \text{s} \times 0.835 = 4,175 \text{ n/cm}^2 / \text{s}$$

Initial neutron flux rate reduced from $5,000 \text{ n/cm}^2 / \text{s}$ to $4,175 \text{ n/cm}^2 / \text{s}$

The attenuation of the neutron flux by the phantom is about 16%.

Neutron Half-Value Layers in centimeters

| Energy in MeV | 1 | 5 | 10 | 15 |
|---------------|-----|------|------|------|
| Polyethylene | 3.7 | 6.1 | 7.7 | 8.8 |
| Water | 4.3 | 6.9 | 8.8 | 10.1 |
| Concrete | 6.8 | 11 | 14 | 16 |
| Damp soil | 8.8 | 14.3 | 18.2 | 20.8 |

example:

How many half-value layers of polyethylene are needed to attenuate a 100 mRem/hr 5 MeV neutron source to 5 mRem/hr?
How thick does the polyethylene need to be?

$$I = I_0 \times 0.5^n$$

$$I = 5 \text{ mRem/hr}$$

$$I_0 = 100 \text{ mRem/hr}$$

$$n = \text{the number of half-value layers}$$

$$I/I_0 = 0.5^n$$

$$5/100 = 0.05 = 0.5^n$$

$$\ln 0.05 = n \times \ln 0.5$$

$$\ln 0.05/\ln 0.5 = n$$

$$-2.996/-0.693 = n$$

$$4.32 = n$$

It will take 4.32 half-value layers of polyethylene to reduce attenuate the neutron source.

$$4.32 \text{ half-value layers} = 4.32 \times 6.1 \text{ cm} = 26.4 \text{ cm}$$

Exposure Rate in an Air-Filled Ion Chamber

X = $I / m[1 / (2.58E-4 \text{ C} / \text{kg}) - R]$
X = exposure rate (R / sec)
I = current (amperes)
M = mass of air in chamber (kg)

% Resolution of a Gamma Spec System

% R = FWHM / peak energy $\times 100 = \% \text{ resolution}$
FWHM = peak energy width at full width half-max height
peak energy = photopeak energy of interest

True Count Rate Based on the Resolving Time of a Gas-Filled Detector

$R_C = R_O / (1 - R_O Y) = \text{true count rate}$
R_O = observed count rate
Y = resolving time

Specific Gamma-Ray Constant (Γ) for Source Activity (A)

$\Gamma = \varphi E_\gamma (\mu_{\text{en}}/\rho)_{\text{air}} e / W$
 $\Gamma = \text{specific gamma constant (R-cm}^2 / \text{hr-A)}$
 $\varphi = \text{photon fluence rate (}\gamma / \text{cm}^2\text{-hr)}$
 $E_\gamma = \text{gamma photon energy (MeV)}$
 $(\mu_{\text{en}}/\rho) = \text{density thickness of air (g / cm}^2)$
e = electron charge (Coulombs)
W = average amount of energy to produce an ion pair in air (eV)

Dose Rate (D) to Air from a Point Beta Source

D = $300 A / d^2 = \text{rad / hr}$
A = source activity in curies
d = distance from source in feet

Photon Fluence Rate ϕ from a Point Source

$\Phi = AY / 4\pi D^2$ = photon fluence rate ($\gamma / \text{cm}^2\text{-hr}$)
 A = source activity (decay per hr)
 Y = photon yield (γ / decay)
 D = distance from point source (cm)

Exposure Rate (X) from a Point Source

$X (\text{R/hr}) = \Gamma A / D^2$
 Γ = specific gamma ray constant ($\text{R/hr} @ 1 \text{ meter per Ci}$)
 A = activity of source in curies
 D = distance from source in meters

Exposure Rate (X) from a Line Source

Inside $L / 2$: $X_1 (D_1) = X_2 (D_2)$
 Outside $L / 2$: $X_1 (D_1)^2 = X_2 (D_2)^2$
 D_1 = distance from source at location 1
 D_2 = distance from source at location 2
 L = length of line

Note that outside of $L / 2$ the equation is the same as the inverse square law.

Exposure Rate (X) from a Disk Source

$X (\text{R/hr}) = \pi R^2 A_a \Gamma \times \ln[(R^2 + D^2) / D^2] / R^2$
 Γ = $\text{R/hr} @ 1 \text{ meter per Ci}$
 A_a = activity per unit area (curies per sq. meter)
 R = radius of source surface in meters
 D = distance from source surface in meters

Simplify the formula by canceling the R^2 's

$$X (\text{R/hr}) = \pi A_a \Gamma \times \ln[(R^2 + D^2) / D^2]$$

Inverse Square Law

$$X_1 (D_1)^2 = X_2 (D_2)^2$$

X_1 = Measured exposure rate

D_1 = Distance from source for the measured exposure rate

X_2 = Exposure rate to be calculated

D_2 = New distance from the source

Applying the Inverse Square Law to Dose Reduction

Given: A high activity source at an unknown distance.

Find: Exposure rate from the source at 30 cm without approaching closer to the source.

X_1 is measured exposure rate at distance Y

X_2 is measured exposure rate at distance $Y + 100$ cm

$$X_1 (Y)^2 = X_2 (Y + 100 \text{ cm})^2$$

$$Y^2 = X_2 (Y + 100 \text{ cm})^2 / X_1$$

Set up this equation by entering the exposure rates you measured at distances Y and $Y + 100$ cm.

Let us assume 100 mr/hr and 50 mr/hr for those two points.

$$Y^2 = 50 (Y + 100 \text{ cm})^2 / 100 = 0.5Y^2 + 100Y + 5,000$$

$$\text{simplify this to } Y^2 - 200Y - 10,000 = 0$$

This quadratic equation can be factored into two answers.

The positive answer for Y is 241.42 cm.

Now we know the distance for exposure rate X_2 and we can calculate the exposure rate at any distance.

The exposure rate at 30 cm would be 6,476 mR/hr but we were able to calculate that exposure rate without entering the High Radiation Area.

A simpler method without having to factor a quadratic equation is to back AWAY from the source until the exposure rate is $\frac{1}{4}$ of the initial rate. The distance you moved away is equal to the original distance to the source. Now you can use the inverse square law to calculate the 30 cm exposure rate.

A comparison of signal levels for various counting gases

| Counting Gas | ω Factor eV / ion pair | Gas Density (g / L) |
|--|----------------------------------|------------------------|
| Air | 33.8 | 1.2928 |
| Ar | 26.4 | 1.8 |
| He | 41.3 | 0.183 |
| H ₂ | 36.5 | 0.09 |
| N ₂ | 34.8 | 1.25 |
| O ₂ | 30.8 | 1.43 |
| CH ₄ | 27.3 | 0.717 |
| Ne | 36.2 | 0.9 |
| Xe | 21.5 | 5.9 |
| Ne + 0.5 % Ar | 25.3 | 0.909 |
| Ar + 0.5 % C ₂ H ₂ | 20.3 | 1.75 |
| Ar + 0.8 % CH ₄ | 26.0 | 1.78 |
| Ar + 10 % CH ₄ (P-10) | 26.0 | 1.616 |

Use this equation to calculate the current flow in femto-amps for an ion chamber at 1 mR/hr exposure rate.

$$0.871 \times V \times P \times \text{fill gas g / l} / (T \times \omega \text{ for fill gas})$$

where; V is chamber volume in cc,

P is chamber pressure in mm Hg,

T is $273.15 + {}^{\circ}\text{C}$,

fill gas density in grams per liter,

ω for fill gas

Table 1 of DOE 5400.5

| Radionuclides | Surface Activity Guidelines | | |
|--|------------------------------------|------------|------------------|
| | Ave | Max | Removable |
| Group 1: Transuranics, I-125, I-129, Ac-227, Ra-226, Ra-228, Th-228, Th-230, Pa-231 | 100 | 300 | 20 |
| Group 2: Th-natural, Sr-90, I-126, I-131, I-133, Ra-223, Ra-224, U-232, Th-232 | 1,000 | 3,000 | 200 |
| Group 3: U-natural, U-235, U-238, and associated decay products, alpha emitters | 5,000 | 15,000 | 1,000 |
| Group 4: Beta/gamma emitters ¹ | 5,000 | 15,000 | 1,000 |
| Tritium² | N/A | N/A | 10,000 |

¹ radionuclides with decay modes other than alpha emission or spontaneous fission except Sr-90 and others noted above

² applicable to surface and subsurface

Appendix D of 10CFR835

| Nuclide | Removable | Total (fixed + removable) |
|--|------------------|----------------------------------|
| Natural U, U-235, U-238, and associated decay products | 1,000 alpha | 5,000 alpha |
| Transuranics , Ra-226, Ra-228, Th-230, Th-228, Pa-231, Ac-227, I-125, I-129 | 20 | 500 |
| Natural Th , Th-232, Sr-90, Ra-223, Ra-224, U-232, I-126, I-131, I-133 | 200 | 1,000 |
| Beta/gamma emitters ¹ | 1,000 | 5,000 |
| Tritium² | 10,000 | 10,000 |

¹ nuclides with decay modes other than alpha emission or spontaneous fission except 90Sr and others noted above

² Tritium organic compounds, surfaces contaminated by HT, HTO, and metal tritide aerosols

Contamination levels in dpm/100 cm²

INSTRUMENT SELECTION AND USE

Exposure/Absorbed Dose Rates (photon) - Ion Chamber, Energy Compensated GM, Tissue-Equivalent Plastic

Dose Equivalent Rates (neutron) - BF₃ or He³ moderator, Neutron-Proton Recoil (Rossi Detector, Liquid Plastic

Scintillator, Plastic/ZnS Scintillator) , LiGdBO₃-loaded Plastic

Beta and activity - Proportional Counter, GM, Plastic Scintillator

Alpha activity - Proportional Counter, ZnS Scintillator, Air Proportional, Solid-state Silicon, Plastic Scintillator

Alpha + beta activity - Proportional Counter, Plastic/ZnS Scintillator, Plastic Scintillator, Solid-state Silicon

Gross gamma activity - NaI, CsI

X-ray spectroscopy - Si(Li)

Gamma spectroscopy - HPGe, CZT, HgI, CsI, LaBr

Alpha spectroscopy - Frisch Grid, Solid-state Silicon

Beta spectroscopy - BGO, Plastic Scintillator, Silicon

1. Select an instrument appropriate for the isotope(s) to be surveyed for.
2. Check instrument for a valid calibration sticker and for damage that would prevent it (them) from operating acceptably.
3. Check the battery condition.
4. Perform an operational (or performance) check.
5. Determine the isotope(s) correction factor to be applied to the instrument.
6. Calculate the instrument's MDA and compare to survey criteria.
7. If the instrument does not meet all of the above criteria, then replace the instrument (or change/charge the batteries) or change your survey technique so that the instrument's MDA will meet the survey criteria.
9. Perform and then document the survey.

6CEN

The 6CEN equation can be used to calculate the exposure rate in R/hr at one foot for x-ray and gamma radiation point sources with energies between 70 KeV and 2 MeV.

$$\text{R/hr at 1 foot} = \text{6CEN}$$

where; C = curies of radioactive material

E = photon energy in MeV

N = abundance of that photon expressed as a decimal

1.6TBqEN

The same formula in Sv/h is given by 1.6 TBqEN, where TBq is the number of terabecquels.

$$\text{Sv/hr at 30 cm} = 1.6\text{TBqEN}$$

where; TBq = quantity of radioactive material

Airborne Activity General Dispersion Model

Assume a 1 μCi (37 kBq) release of respirable Pu-239 inside a large room measuring 12 x 12 x 3 meters with a ventilation turnover rate of 7 volumes per hour. The General Dispersion Model uses this 3D formula for volume. $V = \frac{2}{3} \times \pi \times R^3$

| | | | |
|-------------------------|--------|--------|--------|
| Volume in cm^3 | 30 cm | 1 M | 10 M |
| @ distance R | 5.65E4 | 2.09E6 | 2.09E9 |

Concentration @ distance R

| | | | |
|-------------------------------|---------|---------|----------|
| in $\mu\text{Ci} / \text{cc}$ | 1.77E-5 | 4.78E-7 | 4.78E-10 |
| in Bq / M^3 | 6.55E5 | 1.77E4 | 17.7 |
| in DAC | 8.85E6 | 2.39E5 | 239 |

Time for airborne wave front to reach distance R

| | | |
|--------|--------|----------|
| 13 sec | 43 sec | 7.15 min |
|--------|--------|----------|

1 CFM sample for 1 week equals 10,080 CF (285.4 M^3)

2 CFM sample for 1 week equals 20,160 CF (571 M^3)

Airborne Radioactivity (long-lived)

$C_S = R_N / (V \times \epsilon \times SA \times CE \times CF)$
 C_S = activity concentration at end of sample run time
 R_N = net counting rate
 V = sample volume
 ϵ = detector efficiency
 SA = self-absorption factor
 CE = collection efficiency
 CF = conversion from disintegrations per unit time to activity

Airborne Radioactivity (short-lived)

$C_S = R_N / [V \times \epsilon \times SA \times CE \times CF \times (1 - e^{-\lambda t_s}) \times (e^{-\lambda t_d})]$
 t_s = sample count time
 t_d = time elapsed between end of sample run time and start of sample count time

RESPIRATORY PROTECTION FACTORS (PF) 10CFR20

| Device | Mode | Particulates | Vapors | PF |
|-------------------------|------|--------------|--------|--------|
| Air-purifying half-mask | D | Y | N | 10 |
| Air-purifying full-face | D | Y | N | 50 |
| Air-purifying full-face | PP | Y | N | 1000 |
| Supplied-air hood | PP | Y | Y | 1000* |
| Supplied-air full-face | PP | Y | Y | 2000 |
| SCBA | D | Y | N | 50 |
| SCBA | PD | Y | Y | 10,000 |

* 2000 for supplied-air hood if run at max flow with calibrated flow gauge.

Bubble suits have been used in Pu atmospheres as high as 1,000,000 DAC. Supplied-air respirators are worn inside the bubble suits and real-time air monitoring INSIDE the bubble suits is performed.

Ventilation Rates


Ventilation rates of work areas for health physics and industrial hygiene requirements is typically 6 to 7 volume turnovers per hour.

Calculate the ventilation rate in CFM to ventilate a room at 7 volume turnovers per hour given room dimensions of 30 feet by 30 feet by 10 feet. Volume of the room is $30 \times 30 \times 10 = 9,000$ cubic feet. Seven volume turnovers per hour would be 7 times 9,000 cubic feet or 63,000 cubic feet per hour (1,050 CFM) room ventilation rate.

Lung Deposition from ICRP 30

| AMAD | NP | TB | |
|-------|--------------|------------------|----------|
| μ | Naso-pharanx | Trachea-bronchus | Alveolar |
| 0.1 | 0.01 | 0.08 | 0.61 |
| 1 | 0.3 | 0.08 | 0.25 |
| 10 | 0.9 | 0.08 | 0.04 |

Regions of Deposition

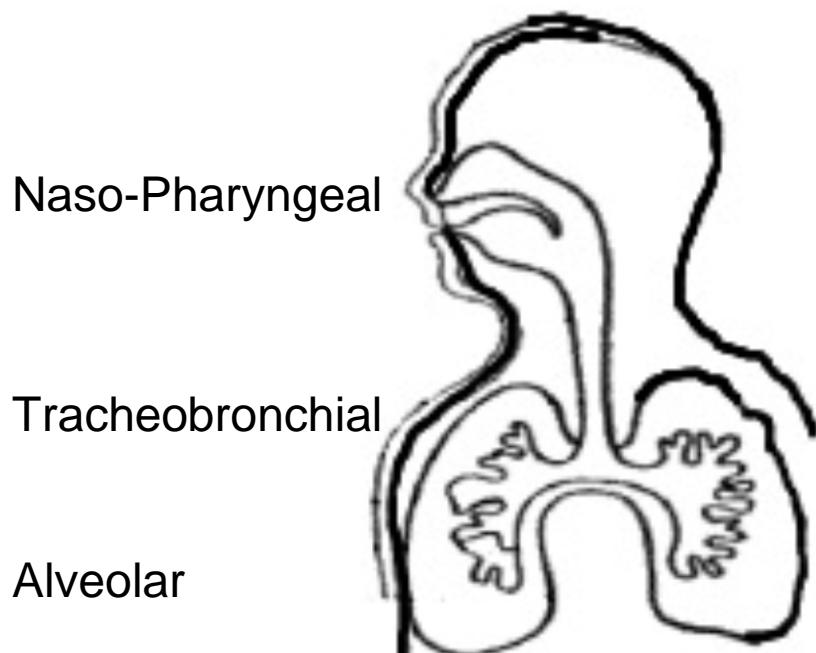

AIR MONITORING

Concentration

Concentration is activity per volume of air and may be stated as dpm / cubic meter, μCi / ml, or Bq / cubic meter. DAC (Derived Air Concentration) is another way to express airborne radioactivity concentrations as relative hazards.

| | | |
|------------------------------|---|--|
| DPM | = | Sample CPM / Eff (CPM / DPM) |
| $1 \mu\text{Ci}$ | = | 2.22×10^6 DPM |
| $1 \text{ DPM} / \text{m}^3$ | = | $4.5 \times 10^{-13} \mu\text{Ci} / \text{ml}$ |
| $1 \mu\text{Ci} / \text{ml}$ | = | $2.22 \times 10^{12} \text{ DPM} / \text{m}^3$ |
| 1 Bq | = | 1 DPS |
| DPM / m^3 | = | $\text{CPM}/(\text{Eff} \times \text{total sample volume in m}^3)$ |
| $\mu\text{Ci} / \text{ml}$ | = | $\text{CPM}/(\text{Eff} \times 2.22 \times 10^6 \text{ DPM} / \mu\text{Ci} \times \text{total sample volume in ml})$ |
| Bq / m^3 | = | $\text{CPM} / (\text{Eff} \times 60 \text{ DPM} / \text{Bq} \times \text{total sample volume in m}^3)$ |
| DAC | = | $\mu\text{Ci} / \text{ml}$ ($\mu\text{Ci} / \text{ml}$ per DAC {DAC Factor}) |
| 1 DAC-h | = | 1 DAC exposure for 1 hour |
| 1 DAC-h | = | 2.5 mrem = 25 μSv |

Calculate the number of DAC-h on a filter by this formula

$$\# \text{ DAC-h} = \# \text{ of DPM on filter} / (\text{Sample LPM} \times 1.332 \times 10^{11} \times \text{DAC factor})$$

Calculate the DPM on a filter to reach 8 DAC-h

$$\text{DPM} = 8 \text{ DAC-h} \times \text{LPM} \times 1.332 \times 10^{11} \times \text{DAC factor}$$

Calculate the DAC level on a filter from the # of DPM

$$\text{DAC} = \# \text{ of DPM} / (\text{DAC factor} \times \text{LPM} \times \text{time in minutes} \times 2.22 \times 10^9)$$

AIR FLOW METER CORRECTIONS

Mass Flow Meters

$$Q_S = Q_A (P_A / P_S \times T_S / T_A)$$

$$Q_A = Q_S (P_S / P_A \times T_A / T_S)$$

where; Q_S is the STP flow rate

Q_A is the ambient flow rate

P_S is STP pressure

P_A is the ambient pressure

T_S is STP temperature

T_A is the ambient temperature

Rotameter Corrections

$$Q_S = Q_I \times P_S / P_A \times T_S / T_A / \sqrt{(P_S / P_I \times T_A / T_S)}$$

where; Q_I is the rotameter flow indication

P_I is the actual pressure inside the rotameter.

This correction assumes the rotameter markings are correct at STP. The actual pressure inside the rotameter should be used in the calculations.

NOTE: A specific class of rotameter known as a “bypass” flowmeter remains correct regardless of the actual barometric pressure.

For personnel protection against particulate airborne radioactivity ambient sample volumes instead of volumes corrected to STP should be used for calculations. The ambient respiratory rate will remain the same as atmospheric pressure changes from STP up to an elevation of approximately 12,000 feet (3,660 Meters).

Filter Media Characteristics for Alpha CAMs

| Filter Type | Pore Size | Filter DP | FWHM keV |
|----------------------|-----------|-----------|----------|
| Millipore | | | |
| Fluoropore | 5 μ | 0.5"Hg | 370 |
| Fluoropore | 3 μ | 0.8"Hg | 300 |
| SMWP | 5 μ | 2.0"Hg | 450 |
| SSWP | 3 μ | 3.1"Hg | 350 |
| AW19 | 1.2 μ | 3.8"Hg | 450 |
| Durapore | 5 μ | 4.3"Hg | 490 |
| AP40 | 0.7 μ | 2.6"Hg | 490 |
| Bladewerx | | | |
| Speclon 1.5 | 1.5 μ | 2.6"Hg | 300 |
| Speclon 5.0 | 5 μ | 0.4"Hg | 370 |
| Whatman | | | |
| GFA | 0.3 μ | 2.8"Hg | 490 |
| EPM 2000 | 0.6 μ | 1.8"Hg | 1,000 |
| Gelman | | | |
| A/E Glass | 1.0 μ | 2.3"Hg | 1,000 |
| Versapor 3000 | 3.0 μ | 2.3"Hg | 450 |
| Hollingsworth & Vose | | | |
| HV LB5211 | 0.3 μ | 1.0"Hg | 650 |

The rated pore size is for >99.99% collection efficiency for that size particle and greater. All of these filters have >99% collection efficiency for particles as small as 0.3 μ m. The stated pressure drop is for a 40 mm collection diameter with an air flow rate of 2 ACFM and barometric pressure of 23.1"Hg. The FWHM is for Po-214 at 7.68 MeV and was determined using a 25 mm collection diameter and a 25 mm diameter diffused junction detector with a spacing of 4 mm. The pressure drop will be higher and the FWHM will be broader at higher barometric pressures.

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL Bq/M³ | | 10CFR20 ALIs uCi | |
|-----------------------|-------------------------------------|---|------------|-------------------------|------|
| | | Ingestion | Inhalation | | |
| H-3 ¹ | X | 2E-05 | 7E+5 | X | X |
| H-3 ² | X | 2E-01 | 9E+9 | X | X |
| H-3 ³ | 2E-05 | X | X | 8E+4 | 8E+4 |
| STCs ⁴ | X | 2E-06 | 8E+4 | X | X |
| STCs ⁵ | X | 1E-05 | 5E+5 | X | X |
| Be-7 | 8E-06 | 1E-05 | 4E+5 | 4E+4 | 2E+4 |
| Be-10 | 6E-09 | 2E-08 | 1E+3 | 1E+3 | 2E+2 |
| C-11 ^{6, 38} | X | 1E-04 | 6E+6 | X | X |
| C-11 ⁷ | 5E-04 | 4E-04 | 1E+7 | X | 1E+6 |
| C-11 ⁸ | 3E-04 | 2E-04 | 9E+6 | X | 6E+5 |
| C-11 ⁹ | 2E-04 | X | X | 4E+5 | 4E+5 |
| C-14 ⁶ | X | 9E-07 | 3E+4 | X | X |
| C-14 ⁷ | 7E-04 | 7E-04 | 2E+7 | X | 2E+6 |
| C-14 ⁸ | 9E-05 | 8E-05 | 3E+6 | X | 2E+5 |
| C-14 ⁹ | 1E-06 | X | X | 2E+3 | 2E+3 |
| F-18 ³⁸ | 3E-05 | 3E-06 | 1E+5 | 5E+4 | 7E+4 |
| Na-22 | 3E-07 | 2E-07 | 1E+4 | 4E+2 | 6E+2 |
| Na-24 | 2E-06 | 4E-07 | 1E+4 | 4E+3 | 5E+3 |
| Mg-28 | 5E-07 | 3E-07 | 1E+4 | 7E+2 | 1E+3 |
| Al-26 | 3E-08 | 4E-08 | 1E+3 | 4E+2 | 60 |
| Si-31 | 1E-06 | 5E-06 | 1E+5 | 9E+3 | 3E+4 |
| Si-32 | 2E-09 | 1E-08 | 3E+2 | 2E+3 | 5 |
| P-32 | 2E-07 | 5E-07 | 7E+3 | 6E+2 | 4E+2 |
| P-33 | 1E-06 | 4E-06 | 1E+4 | 6E+3 | 3E+3 |
| S-35 ¹⁰ | 6E-06 | 4E-06 | 1E+5 | X | 1E+4 |
| S-35 | 9E-07 | 5E-07 | 1E+4 | 6E+3 | 2E+3 |
| Cl-36 | 1E-07 | 1E-07 | 4E+3 | 2E+3 | 2E+2 |
| Cl-38 ³⁸ | 2E-05 | 5E-06 | 2E+5 | 2E+4 | 4E+4 |
| Cl-39 ³⁸ | 2E-05 | 2E-06 | 1E+5 | 2E+4 | 5E+4 |
| K-40 | 2E-07 | 1E-07 | 6E+3 | 3E+2 | 4E+2 |

| | 10CFR20 DAC µCi/mL | 10CFR835 DAC µCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| K-42 ³⁸ | 2E-06 | 2E-06 | 1E+5 | 5E+3 | 5E+3 |
| K-43 | 4E-06 | 9E-07 | 3E+4 | 6E+3 | 9E+3 |
| K-44 | 3E-05 | 8E-06 | 2E+5 | 2E+4 | 7E+4 |
| K-45 ³⁸ | 5E-05 | 9E-06 | 3E+5 | 3E+4 | 1E+5 |
| Ca-41 | 2E-06 | 2E-06 | 8E+4 | 3E+3 | 4E+3 |
| Ca-45 | 4E-07 | 2E-07 | 9E+3 | 2E+3 | 8E+2 |
| Ca-47 | 4E-07 | 2E-07 | 9E+3 | 8E+2 | 9E+2 |
| Sc-43 | 9E-06 | 2E-06 | 7E+4 | 7E+3 | 2E+4 |
| Sc-44m | 3E-07 | 2E-07 | 1E+4 | 5E+2 | 7E+2 |
| Sc-44 | 5E-06 | 1E-06 | 4E+4 | 4E+3 | 1E+4 |
| Sc-46 | 1E-07 | 1E-07 | 4E+3 | 9E+2 | 2E+2 |
| Sc-47 | 1E-06 | 7E-07 | 2E+4 | 2E+3 | 3E+3 |
| Sc-48 | 6E-07 | 2E-07 | 1E+4 | 8E+2 | 1E+3 |
| Sc-49 ³⁸ | 2E-05 | 8E-06 | 3E+5 | 2E+4 | 5E+4 |
| Ti-44 | 2E-09 | 7E-09 | 2E+2 | 3E+2 | 6 |
| Ti-45 | 1E-05 | 2E-06 | 1E+5 | 9E+3 | 3E+4 |
| V-47 ³⁸ | 3E-05 | 6E-06 | 2E+5 | 3E+4 | 8E+4 |
| V-48 | 3E-07 | 2E-07 | 7E+3 | 6E+2 | 6E+2 |
| V-49 | 8E-06 | 1E-05 | 7E+5 | 7E+4 | 2E+4 |
| Cr-48 | 3E-06 | 2E-06 | 8E+4 | 6E+3 | 7E+3 |
| Cr-49 ³⁸ | 4E-05 | 5E-06 | 2E+5 | 3E+4 | 8E+4 |
| Cr-51 | 8E-06 | 1E-05 | 5E+5 | 4E+4 | 2E+4 |
| Mn-51 ³⁸ | 2E-05 | 7E-06 | 2E+5 | 2E+4 | 5E+4 |
| Mn-52m ³⁸ | 4E-05 | 5E-06 | 2E+5 | 3E+4 | 9E+4 |
| Mn-52 | 4E-07 | 2E-07 | 8E+3 | 7E+2 | 9E+2 |
| Mn-53 | 5E-06 | 1E-05 | 2E+5 | 5E+4 | 1E+4 |
| Mn-54 | 3E-07 | 4E-07 | 1E+4 | 2E+3 | 8E+2 |
| Mn-56 | 6E-06 | 2E-06 | 8E+4 | 5E+3 | 2E+4 |
| Fe-52 | 1E-06 | 5E-07 | 2E+4 | 9E+2 | 2E+3 |
| Fe-55 | 8E-07 | 6E-07 | 2E+4 | 9E+3 | 2E+3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|----------------------|-------------------------------------|--------------------------------------|-------------------------|------------------------------------|
| | | | | Ingestion Inhalation |
| Fe-59 | 1E-07 | 1E-07 | 6E+3 | 8E+2 3E+2 |
| Fe-60 | 3E-09 | 1E-09 | 60 | 30 6 |
| Co-55 | 1E-06 | 5E-07 | 2E+4 | 1E+3 3E+3 |
| Co-56 | 8E-08 | 1E-07 | 4E+3 | 4E+2 2E+2 |
| Co-57 | 3E-07 | 9E-07 | 3E+4 | 4E+3 7E+2 |
| Co-58m | 3E-05 | 3E-05 | 1E+6 | 6E+4 6E+4 |
| Co-58 | 3E-07 | 3E-07 | 1E+4 | 1E+3 7E+2 |
| Co-60m ³⁸ | 1E-03 | 4E-04 | 1E+7 | 1E+6 3E+6 |
| Co-60 | 1E-08 | 3E-08 | 1E+3 | 2E+2 30 |
| Co-61 ³⁸ | 2E-05 | 6E-06 | 2E+5 | 2E+4 6E+4 |
| Co-62m ³⁸ | 6E-05 | 6E-06 | 2E+5 | 4E+4 2E+5 |
| Ni-56 | 5E-07 | X | X | 1E+3 1E+3 |
| Ni-56 ¹¹ | X | 4E-07 | 1E+4 | X X |
| Ni-56 ¹² | X | 4E-07 | 1E+4 | X X |
| Ni-57 | 1E-06 | X | X | 2E+3 3E+3 |
| Ni-57 ¹¹ | X | 5E-07 | 2E+4 | X X |
| Ni-57 ¹² | X | 7E-07 | 2E+4 | X X |
| Ni-59 | 8E-07 | X | X | 2E+4 2E+3 |
| Ni-59 ¹¹ | X | 2E-06 | 9E+4 | X X |
| Ni-59 ¹² | X | 6E-07 | 2E+4 | X X |
| Ni-63 | 3E-07 | X | X | 9E+3 2E+3 |
| Ni-63 ¹¹ | X | 1E-06 | 4E+4 | X X |
| Ni-63 ¹² | X | 2E-07 | 1E+4 | X X |
| Ni-65 | 7E-06 | X | X | 8E+3 2E+4 |
| Ni-65 ¹¹ | X | 4E-06 | 1E+5 | X X |
| Ni-65 ¹² | X | 8E-07 | 3E+4 | X X |
| Ni-66 | 3E-07 | X | X | 4E+2 6E+2 |
| Ni-66 ¹¹ | X | 2E-07 | 1E+4 | X X |
| Ni-66 ¹² | X | 2E-07 | 1E+4 | X X |
| Cu-60 ³⁸ | 4E-05 | 4E-06 | 1E+5 | 3E+4 9E+4 |

| | 10CFR20 DAC µCi/mL | 10CFR835 DAC µCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|---------------------|-------------------------------------|--------------------------------------|-------------------------|------------------------------------|
| | | | | Ingestion Inhalation |
| Cu-61 | 1E-05 | 3E-06 | 1E+5 | 1E+4 3E+4 |
| Cu-64 | 9E-06 | 3E-06 | 1E+5 | 1E+4 2E+4 |
| Cu-67 | 2E-06 | 2E-06 | 3E+4 | 5E+3 5E+3 |
| Zn-62 | 1E-06 | 9E-07 | 3E+4 | 1E+3 3E+3 |
| Zn-63 ³⁸ | 3E-05 | 8E-07 | 2E+5 | 2E+4 7E+4 |
| Zn-65 | 1E-07 | 5E-06 | 7E+3 | 4E+2 3E+2 |
| Zn-69m | 3E-06 | 2E-07 | 6E+4 | 4E+3 7E+3 |
| Zn-69 ³⁸ | 6E-05 | 1E-06 | 2E+5 | 6E+4 1E+5 |
| Zn-71m | 7E-06 | 7E-06 | 5E+4 | 6E+3 2E+4 |
| Zn-72 | 5E-07 | 1E-06 | 1E+4 | 1E+3 1E+3 |
| Ga-65 ³⁸ | 7E-05 | 3E-07 | 3E+5 | 5E+4 2E+5 |
| Ga-66 | 1E-06 | 7E-07 | 2E+4 | 1E+3 3E+3 |
| Ga-67 | 4E-06 | 2E-06 | 7E+4 | 7E+3 1E+4 |
| Ga-68 ³⁸ | 2E-05 | 4E-06 | 1E+5 | 2E+4 4E+4 |
| Ga-70 ³⁸ | 7E-05 | 1E-05 | 4E+5 | 5E+4 2E+5 |
| Ga-72 | 1E-06 | 5E-07 | 2E+4 | 1E+3 3E+3 |
| Ga-73 | 6E-06 | 2E-06 | 1E+5 | 5E+3 2E+4 |
| Ge-66 | 8E-06 | 2E-06 | 9E+4 | 2E+4 2E+4 |
| Ge-67 ³⁸ | 4E-05 | 7E-06 | 2E+5 | 3E+4 9E+4 |
| Ge-68 | 4E-08 | 7E-08 | 2E+3 | 5E+3 1E+2 |
| Ge-69 | 3E-06 | 1E-06 | 3E+4 | 1E+4 8E+3 |
| Ge-71 | 2E-05 | 5E-05 | 1E+6 | 5E+5 4E+4 |
| Ge-75 ³⁸ | 3E-05 | 7E-06 | 2E+5 | 4E+4 8E+4 |
| Ge-77 | 2E-06 | 1E-06 | 4E+4 | 9E+3 6E+3 |
| Ge-78 ³⁸ | 9E-06 | 3E-06 | 1E+5 | 2E+4 2E+4 |
| As-69 ³⁸ | 5E-05 | 9E-06 | 3E+5 | 3E+4 1E+5 |
| As-70 ³⁸ | 2E-05 | 2E-06 | 8E+4 | 1E+4 5E+4 |
| As-71 | 2E-06 | 1E-06 | 4E+4 | 4E+3 5E+3 |
| As-72 | 6E-07 | 4E-07 | 1E+4 | 9E+2 1E+3 |
| As-73 | 7E-07 | 8E-07 | 3E+4 | 8E+3 2E+3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|----------------------|-------------------------------------|--------------------------------------|-------------------------|----------------------------------|
| | | | | Ingestion Inhalation |
| As-74 | 3E-07 | 3E-07 | 1E+4 | 1E+3 8E+2 |
| As-76 | 6E-07 | 6E-07 | 2E+4 | 1E+3 1E+3 |
| As-77 | 2E-06 | 1E-06 | 4E+4 | 4E+3 5E+3 |
| As-78 ³⁸ | 9E-06 | 3E-06 | 1E+5 | 8E+3 2E+4 |
| Se-70 ³⁸ | 2E-05 | 2E-06 | 9E+4 | 1E+4 4E+4 |
| Se-73m ³⁸ | 6E-05 | 1E-05 | 4E+5 | 3E+4 1E+5 |
| Se-73 | 5E-06 | 1E-06 | 5E+4 | 3E+3 1E+4 |
| Se-75 | 3E-07 | 3E-07 | 1E+4 | 5E+2 6E+2 |
| Se-79 | 2E-07 | 1E-07 | 6E+3 | 6E+2 6E+2 |
| Se-81m ³⁸ | 3E-05 | 6E-06 | 2E+5 | 2E+4 7E+4 |
| Se-81 ³⁸ | 9E-05 | 1E-05 | 4E+5 | 6E+4 2E+5 |
| Se-83 ³⁸ | 5E-05 | 5E-06 | 1E+5 | 3E+4 1E+5 |
| Br-74m ³⁸ | 2E-05 | 2E-06 | 1E+5 | 1E+4 4E+4 |
| Br-74 ³⁸ | 3E-05 | 4E-06 | 1E+5 | 2E+4 7E+4 |
| Br-75 ³⁸ | 2E-05 | 3E-06 | 1E+5 | 3E+4 5E+4 |
| Br-76 | 2E-06 | 5E-07 | 2E+4 | 4E+3 4E+3 |
| Br-77 | 8E-06 | 2E-06 | 7E+4 | 2E+4 2E+4 |
| Br-80m | 6E-06 | 5E-06 | 2E+5 | 2E+4 1E+4 |
| Br-80 ³⁸ | 8E-05 | 2E-05 | 7E+5 | 5E+4 2E+5 |
| Br-82 | 2E-06 | 3E-07 | 1E+4 | 3E+3 4E+3 |
| Br-83 | 3E-05 | 6E-06 | 2E+5 | 5E+4 6E+4 |
| Br-84 ³⁸ | 2E-05 | 5E-06 | 2E+5 | 2E+4 6E+4 |
| Rb-79 ³⁸ | 5E-05 | 8E-06 | 2E+5 | 4E+4 1E+5 |
| Rb-81m ³⁸ | 1E-04 | 1E-05 | 6E+5 | 2E+5 3E+5 |
| Rb-81 | 2E-05 | 2E-06 | 1E+5 | 4E+4 5E+4 |
| Rb-82m | 7E-06 | 8E-07 | 3E+4 | 1E+4 2E+4 |
| Rb-83 | 4E-07 | 5E-07 | 2E+4 | 6E+2 1E+3 |
| Rb-84 | 3E-07 | 3E-07 | 1E+4 | 5E+2 8E+2 |
| Rb-86 | 3E-07 | 4E-07 | 1E+4 | 5E+2 8E+2 |
| Rb-87 | 6E-07 | 7E-07 | 2E+4 | 1E+3 2E+3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| Rb-88 ³⁸ | 3E-05 | 1E-05 | 5E+5 | 2E+4 | 6E+4 |
| Rb-89 ³⁸ | 6E-05 | 1E-05 | 3E+5 | 4E+4 | 1E+5 |
| Sr-80 ³⁸ | 5E-06 | 2E-06 | 9E+4 | 4E+3 | 1E+4 |
| Sr-81 ³⁸ | 3E-05 | 5E-06 | 2E+5 | 2E+4 | 8E+4 |
| Sr-82 | 4E-08 | 7E-08 | 2E+3 | 2E+2 | 90 |
| Sr-83 | 1E-06 | 9E-07 | 3E+4 | 2E+3 | 4E+3 |
| Sr-85m ³⁸ | 3E-04 | 3E-05 | 1E+6 | 2E+5 | 6E+5 |
| Sr-85 | 6E-07 | 8E-07 | 3E+4 | 3E+3 | 2E+3 |
| Sr-87m | 5E-05 | 9E-06 | 3E+5 | 4E+4 | 1E+5 |
| Sr-89 | 6E-08 | 1E-07 | 3E+3 | 5E+2 | 1E+2 |
| Sr-90 | 2E-09 | 7E-09 | 2E+2 | 30 | 4 |
| Sr-91 | 1E-06 | 9E-07 | 3E+4 | 2E+3 | 4E+3 |
| Sr-92 | 3E-06 | 1E-06 | 6E+4 | 3E+3 | 7E+3 |
| Y-86m ³⁸ | 2E-05 | 6E-06 | 2E+5 | 2E+4 | 5E+4 |
| Y-86 | 1E-06 | 4E-07 | 1E+4 | 1E+3 | 3E+3 |
| Y-87 | 1E-06 | 8E-07 | 3E+4 | 2E+3 | 3E+3 |
| Y-88 | 1E-07 | 1E-07 | 6E+3 | 1E+3 | 2E+2 |
| Y-90m | 5E-06 | 4E-06 | 1E+5 | 8E+3 | 1E+4 |
| Y-90 | 3E-07 | 3E-07 | 1E+4 | 4E+2 | 6E+2 |
| Y-91m ³⁸ | 7E-05 | 2E-05 | 7E+5 | 1E+5 | 2E+5 |
| Y-91 | 5E-08 | 9E-08 | 3E+3 | 5E+2 | 1E+2 |
| Y-92 | 3E-06 | 2E-06 | 7E+4 | 3E+3 | 8E+3 |
| Y-93 | 1E-06 | 9E-07 | 3E+4 | 1E+3 | 2E+3 |
| Y-94 ³⁸ | 3E-05 | 8E-06 | 3E+5 | 2E+4 | 8E+4 |
| Y-95 ³⁸ | 6E-05 | 1E-05 | 4E+5 | 4E+4 | 1E+5 |
| Zr-86 | 1E-06 | 5E-07 | 2E+4 | 1E+3 | 2E+3 |
| Zr-88 | 9E-08 | 1E-07 | 5E+3 | 4E+3 | 2E+2 |
| Zr-89 | 1E-06 | 6E-07 | 2E+4 | 2E+3 | 2E+3 |
| Zr-93 | 3E-09 | 3E-09 | 1E+2 | 1E+3 | 6 |
| Zr-95 | 5E-08 | 9E-08 | 3E+3 | 1E+3 | 1E+2 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|----------------------|-------------------------------------|--------------------------------------|-------------------------|----------------------------------|
| | | | | Ingestion Inhalation |
| Zr-97 | 5E-07 | 4E-07 | 1E+4 | 6E+2 1E+3 |
| Nb-88 ³⁸ | 9E-05 | 5E-06 | 1E+5 | 5E+4 2E+5 |
| Nb-89m ¹³ | 2E-05 | 3E-06 | 1E+5 | 1E+4 4E+4 |
| Nb-89 ¹⁴ | 6E-06 | 2E-06 | 1E+5 | 5E+3 2E+4 |
| Nb-90 | 1E-06 | 3E-07 | 1E+4 | 1E+3 2E+3 |
| Nb-93m | 7E-08 | 6E-07 | 2E+4 | 9E+3 2E+2 |
| Nb-94 | 6E-09 | 2E-08 | 8E+2 | 9E+2 20 |
| Nb-95m | 9E-07 | 6E-07 | 2E+4 | 2E+3 2E+3 |
| Nb-95 | 5E-07 | 4E-07 | 1E+4 | 2E+3 1E+3 |
| Nb-96 | 1E-06 | 4E-07 | 1E+4 | 1E+3 2E+3 |
| Nb-97 ³⁸ | 3E-05 | 5E-06 | 1E+5 | 2E+4 7E+4 |
| Nb-98 ³⁸ | 2E-05 | 3E-06 | 1E+5 | 1E+4 5E+4 |
| Mo-90 | 2E-06 | 7E-07 | 2E+4 | 2E+3 5E+3 |
| Mo-93m | 6E-06 | 1E-06 | 3E+4 | 4E+3 1E+4 |
| Mo-93 | 8E-08 | 2E-07 | 7E+3 | 2E+4 2E+2 |
| Mo-99 | 6E-07 | 5E-07 | 1E+4 | 1E+3 1E+3 |
| Mo-101 ³⁸ | 6E-05 | 6E-06 | 2E+5 | 4E+4 1E+5 |
| Tc-93m ³⁸ | 6E-05 | 7E-06 | 2E+5 | 3E+4 2E+5 |
| Tc-93 | 3E-05 | 3E-06 | 1E+5 | 3E+4 7E+4 |
| Tc-94m ³⁸ | 2E-05 | 4E-06 | 1E+5 | 2E+4 4E+4 |
| Tc-94 | 8E-06 | 1E-06 | 3E+4 | 9E+3 2E+4 |
| Tc-95m | 8E-07 | 6E-07 | 2E+4 | 4E+3 2E+3 |
| Tc-95 | 8E-06 | 1E-06 | 5E+4 | 1E+4 2E+4 |
| Tc-96m ³⁸ | 1E-04 | 2E-05 | 1E+6 | 2E+5 2E+5 |
| Tc-96 | 9E-07 | 3E-07 | 1E+4 | 2E+3 2E+3 |
| Tc-97m | 5E-07 | 2E-07 | 7E+3 | 5E+3 1E+3 |
| Tc-97 | 2E-06 | 3E-06 | 1E+5 | 4E+4 6E+3 |
| Tc-98 | 1E-07 | 9E-08 | 3E+3 | 1E+3 3E+2 |
| Tc-99m | 6E-05 | 1E-05 | 4E+5 | 8E+4 2E+5 |
| Tc-99 | 3E-07 | 1E-07 | 6E+3 | 4E+3 7E+2 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| Tc-101 ³⁸ | 1E-04 | 1E-05 | 4E+5 | 9E+4 | 3E+5 |
| Tc-104 ³⁸ | 3E-05 | 7E-06 | 2E+5 | 2E+4 | 7E+4 |
| Ru-94 ³⁸ | 2E-05 | 5E-06 | 1E+5 | 2E+4 | 4E+4 |
| Ru-97 | 5E-06 | 2E-06 | 8E+4 | 8E+3 | 1E+4 |
| Ru-103 | 3E-07 | 2E-07 | 9E+3 | 2E+3 | 6E+2 |
| Ru-105 | 5E-06 | 2E-06 | 8E+4 | 5E+3 | 1E+4 |
| Ru-106 | 5E-09 | 1E-08 | 5E+2 | 2E+2 | 10 |
| Rh-99m | 2E-05 | 3E-06 | 1E+5 | 2E+4 | 6E+4 |
| Rh-99 | 8E-07 | 6E-07 | 2E+4 | 2E+3 | 2E+3 |
| Rh-100 | 2E-06 | 5E-07 | 1E+4 | 2E+3 | 4E+3 |
| Rh-101m | 3E-06 | 1E-06 | 6E+4 | 6E+3 | 8E+3 |
| Rh-101 | 6E-08 | 1E-07 | 6E+3 | 2E+3 | 2E+2 |
| Rh-102m | 5E-08 | 1E-07 | 4E+3 | 1E+3 | 1E+2 |
| Rh-102 | 2E-08 | 6E-08 | 2E+3 | 6E+2 | 60 |
| Rh-103m ³⁸ | 5E-04 | 2E-04 | 8E+6 | 4E+5 | 1E+6 |
| Rh-105 | 2E-06 | 1E-06 | 4E+4 | 4E+3 | 6E+3 |
| Rh-106m | 1E-05 | 1E-06 | 5E+4 | 8E+3 | 3E+4 |
| Rh-107 ³⁸ | 1E-04 | 9E-06 | 3E+5 | 7E+4 | 2E+5 |
| Pd-100 | 5E-07 | 5E-07 | 2E+4 | 1E+3 | 1E+3 |
| Pd-101 | 1E-05 | 3E-06 | 1E+5 | 1E+4 | 3E+4 |
| Pd-103 | 1E-06 | 1E-06 | 6E+4 | 6E+3 | 4E+3 |
| Pd-107 | 2E-07 | 1E-06 | 7E+4 | 3E+4 | 4E+2 |
| Pd-109 | 2E-06 | 1E-06 | 4E+4 | 2E+3 | 5E+3 |
| Ag-102 ³⁸ | 8E-05 | 7E-06 | 2E+5 | 5E+4 | 2E+5 |
| Ag-103 ³⁸ | 4E-05 | 7E-06 | 2E+5 | 4E+4 | 1E+5 |
| Ag-104m ³⁸ | 4E-05 | 6E-06 | 2E+5 | 3E+4 | 9E+4 |
| Ag-104 ³⁸ | 3E-05 | 3E-06 | 1E+5 | 2E+4 | 7E+4 |
| Ag-105 | 4E-07 | 7E-07 | 2E+4 | 3E+3 | 1E+3 |
| Ag-106m | 3E-07 | 2E-07 | 9E+3 | 8E+2 | 7E+2 |
| Ag-106 ³⁸ | 8E-05 | 1E-05 | 4E+5 | 6E+4 | 2E+5 |

| | 10CFR20 DAC µCi/mL | 10CFR835 DAC µCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|--------------------------|-------------------------------------|--------------------------------------|-------------------------|------------------------------------|
| | | | | Ingestion Inhalation |
| Ag-108m | 1E-08 | 2E-08 | 1E+3 | 6E+2 20 |
| Ag-110m | 4E-08 | 7E-08 | 2E+3 | 5E+2 90 |
| Ag-111 | 4E-07 | 3E-07 | 1E+4 | 9E+2 9E+2 |
| Ag-112 | 3E-06 | 2E-06 | 8E+4 | 3E+3 8E+3 |
| Ag-115 ³⁸ | 3E-05 | 8E-06 | 3E+5 | 3E+4 8E+4 |
| Cd-104 ³⁸ | 3E-05 | 4E-06 | 1E+5 | 2E+4 7E+4 |
| Cd-107 | 2E-05 | 4E-06 | 1E+5 | 2E+4 5E+4 |
| Cd-109 | 1E-08 | 1E-07 | 9E+2 | 3E+2 50 |
| Cd-113m | 1E-09 | 1E-09 | 60 | 20 2 |
| Cd-113 | 9E-10 | 1E-09 | 50 | 20 2 |
| Cd-115m | 2E-08 | 3E-08 | 1E+3 | 3E+2 50 |
| Cd-115 | 5E-07 | 4E-07 | 1E+4 | 9E+2 1E+3 |
| Cd-117m | 5E-06 | 1E-06 | 4E+4 | 5E+3 1E+4 |
| Cd-117 | 5E-06 | 2E-06 | 7E+4 | 5E+3 1E+4 |
| In-109 | 2E-05 | 4E-06 | 1E+5 | 2E+4 4E+4 |
| In-110 ^{15, 38} | 2E-05 | 4E-06 | 1E+5 | 2E+4 4E+4 |
| In-110 ¹⁶ | 7E-06 | 9E-07 | 3E+4 | 5E+3 2E+4 |
| In-111 | 3E-06 | 1E-06 | 5E+4 | 4E+3 6E+3 |
| In-112 | 3E-04 | 1E-05 | 6E+5 | 2E+5 6E+5 |
| In-113m ³⁸ | 6E-05 | 1E-05 | 3E+5 | 5E+4 1E+5 |
| In-114m | 3E-08 | 5E-08 | 1E+3 | 3E+2 60 |
| In-115m | 2E-05 | 6E-06 | 2E+5 | 1E+4 4E+4 |
| In-115 | 6E-10 | 1E-09 | 40 | 40 10 |
| In-116m ³⁸ | 3E-05 | 4E-06 | 1E+5 | 2E+4 8E+4 |
| In-117m ³⁸ | 1E-05 | 5E-06 | 1E+5 | 1E+4 3E+4 |
| In-117 ³⁸ | 7E-05 | 5E-06 | 2E+5 | 6E+4 2E+5 |
| In-119m ³⁸ | 5E-05 | 1E-05 | 4E+5 | 4E+4 1E+5 |
| Sn-110 | 5E-06 | 1E-06 | 6E+4 | 4E+3 1E+4 |
| Sn-111 ³⁸ | 9E-05 | 1E-05 | 5E+5 | 7E+4 2E+5 |
| Sn-113 | 2E-07 | 2E-07 | 1E+4 | 2E+3 5E+2 |

| | 10CFR20 DAC | 10CFR835 DAC | 10CFR20 ALIs uCi | |
|-----------------------|--------------------|---------------------|-------------------------|-----------------------------|
| | μCi/mL | μCi/mL | Bq/M³ | Ingestion Inhalation |
| Sn-117m | 5E-07 | 2E-07 | 9E+3 | 2E+3 1E+3 |
| Sn-119m | 4E-07 | 3E-07 | 1E+4 | 3E+3 1E+3 |
| Sn-121m | 2E-07 | 1E-07 | 6E+3 | 3E+3 5E+2 |
| Sn-121 | 5E-06 | 2E-06 | 7E+4 | 6E+3 1E+4 |
| Sn-123m ³⁸ | 5E-05 | 7E-06 | 2E+5 | 5E+4 1E+5 |
| Sn-123 | 7E-08 | 1E-07 | 3E+3 | 5E+2 2E+2 |
| Sn-125 | 1E-07 | 2E-07 | 7E+3 | 4E+2 4E+2 |
| Sn-126 | 2E-08 | 3E-08 | 1E+3 | 3E+2 60 |
| Sn-127 | 8E-06 | 2E-06 | 7E+4 | 7E+3 2E+4 |
| Sn-128 ³⁸ | 1E-05 | 2E-06 | 8E+4 | 9E+3 3E+4 |
| Sb-115 ³⁸ | 1E-04 | 1E-05 | 4E+5 | 8E+4 2E+5 |
| Sb-116m ³⁸ | 3E-05 | 2E-06 | 1E+5 | 2E+4 7E+4 |
| Sb-116 ³⁸ | 1E-04 | 1E-05 | 3E+5 | 7E+4 3E+5 |
| Sb-117 | 9E-05 | 1E-05 | 3E+5 | 7E+4 2E+5 |
| Sb-118m | 8E-06 | 1E-06 | 4E+4 | 5E+3 2E+4 |
| Sb-119 | 1E-05 | 6E-06 | 2E+5 | 2E+4 3E+4 |
| Sb-120 ¹⁷ | 2E-04 | 2E-05 | 7E+5 | 1E+5 4E+5 |
| Sb-120 ¹⁸ | 5E-07 | 3E-07 | 1E+4 | 9E+2 1E+3 |
| Sb-122 | 4E-07 | 4E-07 | 1E+4 | 7E+2 1E+3 |
| Sb-124m ³⁸ | 2E-04 | 3E-05 | 1E+6 | 2E+5 6E+5 |
| Sb-124 | 1E-07 | 1E-07 | 4E+3 | 5E+2 2E+2 |
| Sb-125 | 2E-07 | 1E-07 | 6E+3 | 2E+3 5E+2 |
| Sb-126m ³⁸ | 8E-05 | 7E-06 | 2E+5 | 5E+4 2E+5 |
| Sb-126 | 2E-07 | 1E-07 | 6E+3 | 5E+2 5E+2 |
| Sb-127 | 4E-07 | 3E-07 | 1E+4 | 7E+2 9E+2 |
| Sb-128 ¹⁹ | 1E-06 | 5E-07 | 2E+4 | 8E+4 4E+5 |
| Sb-128 ²⁰ | 2E-04 | 9E-06 | 3E+5 | 1E+3 3E+3 |
| Sb-129 | 4E-06 | 1E-06 | 5E+4 | 3E+3 9E+3 |
| Sb-130 ³⁸ | 3E-05 | 2E-06 | 1E+5 | 2E+4 6E+4 |
| Sb-131 ³⁸ | 1E-05 | 4E-06 | 1E+5 | 1E+4 2E+4 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|------------------------------------|
| | | | | Ingestion Inhalation |
| Te-116 | 9E-06 | 2E-06 | 7E+4 | 8E+3 2E+4 |
| Te-116 ¹⁰ | X | 6E-06 | 1E+3 | X X |
| Te-121m | 8E-08 | 1E-07 | 4E+3 | 5E+2 2E+2 |
| Te-121m ¹⁰ | X | 4E-08 | 1E+3 | X X |
| Te-121 | 1E-06 | 1E-06 | 4E+4 | 3E+3 3E+3 |
| Te-121 ¹⁰ | X | 1E-06 | 3E+4 | X X |
| Te-123m | 9E-08 | 1E-07 | 4E+3 | 6E+2 2E+2 |
| Te-123m ¹⁰ | X | 5E-08 | 2E+3 | X X |
| Te-123 | 8E-08 | 2E-08 | 1E+3 | 5E+2 2E+2 |
| Te-123 ¹⁰ | X | 1E-08 | 4E+2 | X X |
| Te-125m | 2E-07 | 1E-07 | 7E+3 | 1E+3 4E+2 |
| Te-125m ¹⁰ | X | 1E-07 | 3E+3 | X X |
| Te-127m | 1E-07 | 9E-08 | 3E+3 | 6E+2 3E+2 |
| Te-127m ¹⁰ | X | 6E-08 | 2E+3 | X X |
| Te-127 | 7E-06 | 3E-06 | 1E+5 | 7E+3 2E+4 |
| Te-127 ¹⁰ | X | 7E-06 | 2E+5 | X X |
| Te-129m | 1E-07 | 1E-07 | 3E+3 | 5E+2 2E+2 |
| Te-129m ¹⁰ | X | 1E-07 | 5E+3 | X X |
| Te-129 ³⁸ | 3E-05 | 7E-06 | 2E+5 | 3E+4 6E+4 |
| Te-129 ¹⁰ | X | 1E-05 | 5E+5 | X X |
| Te-131m | 2E-07 | 3E-07 | 1E+4 | 3E+2 4E+2 |
| Te-131m ¹⁰ | X | 1E-07 | 5E+3 | X X |
| Te-131 ³⁸ | 2E-06 | 7E-06 | 2E+5 | 3E+3 5E+3 |
| Te-131 ¹⁰ | X | 6E-06 | 2E+5 | X X |
| Te-132 | 9E-08 | 1E-07 | 6E+3 | 2E+2 2E+2 |
| Te-132 ¹⁰ | X | 7E-08 | 2E+3 | X X |
| Te-133m ¹⁰ | X | 1E-06 | 6E+4 | X X |
| Te-133m ³⁸ | 2E-06 | 2E-06 | 1E+5 | 3E+3 5E+3 |
| Te-133 ³⁸ | 9E-06 | 9E-06 | 3E+5 | 1E+4 2E+4 |
| Te-133 ¹⁰ | X | 7E-06 | 2E+5 | X X |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|----------------------|-------------------------------------|--------------------------------------|-------------------------|---------------------------|
| | | | | Ingestion Inhalation |
| Te-134 ¹⁰ | X | 6E-06 | 2E+5 | X X |
| Te-134 ³⁸ | 1E-05 | 2E-06 | 1E+5 | 2E+4 2E+4 |
| I-120m ³⁸ | 9E-06 | 2E-06 | 1E+5 | 1E+4 2E+4 |
| I-120m ¹⁰ | X | 3E-06 | 5E+4 | X X |
| I-120m ²¹ | X | 4E-06 | 8E+4 | X X |
| I-120 ³⁸ | 4E-06 | 2E-06 | 6E+4 | 4E+3 9E+3 |
| I-120 ¹⁰ | X | 1E-06 | 5E+4 | X X |
| I-120 ²¹ | X | 1E-06 | 1E+5 | X X |
| I-121 | 8E-06 | 8E-06 | 3E+5 | 1E+4 2E+4 |
| I-121 ¹⁰ | X | 4E-06 | 1E+5 | X X |
| I-121 ²¹ | X | 5E-06 | 2E+5 | X X |
| I-123 | 3E-06 | 2E-06 | 1E+5 | 3E+3 6E+3 |
| I-123 ¹⁰ | X | 1E-06 | 5E+4 | X X |
| I-123 ²¹ | X | 1E-06 | 7E+4 | X X |
| I-124 | 3E-08 | 4E-08 | 1E+3 | 50 80 |
| I-124 ¹⁰ | X | 2E-08 | 9E+2 | X X |
| I-124 ²¹ | X | 3E-08 | 1E+3 | X X |
| I-125 | 3E-08 | 3E-08 | 1E+3 | 40 60 |
| I-125 ¹⁰ | X | 2E-08 | 7E+2 | X X |
| I-125 ²¹ | X | 2E-08 | 9E+2 | X X |
| I-126 | 1E-08 | 2E-08 | 7E+2 | 20 40 |
| I-126 ¹⁰ | X | 1E-08 | 4E+2 | X X |
| I-126 ²¹ | X | 1E-08 | 5E+2 | X X |
| I-128 | 5E-05 | 1E-05 | 6E+5 | 4E+4 1E+5 |
| I-128 ¹⁰ | X | 8E-06 | 3E+5 | X X |
| I-128 ²¹ | X | 3E-05 | 1E+6 | X X |
| I-129 | 4E-09 | 5E-09 | 2E+2 | 50 90 |
| I-129 ¹⁰ | X | 2E-09 | 1E+2 | X X |
| I-129 ²¹ | X | 3E-09 | 1E+2 | X X |
| I-130 | 3E-07 | 3E-07 | 1E+4 | 4E+2 7E+2 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| I-130 ¹⁰ | X | 1E-07 | 6E+3 | X | X |
| I-130 ²¹ | X | 2E-07 | 7E+3 | X | X |
| I-131 | 2E-08 | 2E-08 | 9E+2 | 30 | 50 |
| I-131 ¹⁰ | X | 1E-08 | 5E+2 | X | X |
| I-131 ²¹ | X | 1E-08 | 6E+2 | X | X |
| I-132m ³⁸ | 4E-06 | 3E-06 | 1E+5 | 4E+3 | 8E+3 |
| I-132m ¹⁰ | X | 1E-06 | 6E+4 | X | X |
| I-132m ²¹ | X | 1E-06 | 7E+4 | X | X |
| I-132 | 3E-06 | 2E-06 | 7E+4 | 4E+3 | 8E+3 |
| I-132 ¹⁰ | X | 1E-06 | 5E+4 | X | X |
| I-132 ²¹ | X | 1E-06 | 6E+4 | X | X |
| I-133 | 1E-07 | 1E-07 | 5E+3 | 1E+2 | 3E+2 |
| I-133 ¹⁰ | X | 7E-08 | 2E+3 | X | X |
| I-133 ²¹ | X | 9E-08 | 3E+3 | X | X |
| I-134 ³⁸ | 2E-05 | 3E-06 | 1E+5 | 2E+4 | 5E+4 |
| I-134 ¹⁰ | X | 3E-06 | 1E+5 | X | X |
| I-134 ²¹ | X | 8E-06 | 2E+5 | X | X |
| I-135 | 7E-07 | 6E-07 | 2E+4 | 8E+2 | 2E+3 |
| I-135 ¹⁰ | X | 3E-07 | 1E+4 | X | X |
| I-135 ²¹ | X | 4E-07 | 1E+4 | X | X |
| Cs-125 ³⁸ | 6E-05 | 1E-05 | 4E+5 | 5E+4 | 1E+5 |
| Cs-127 | 4E-05 | 4E-06 | 1E+5 | 6E+4 | 9E+4 |
| Cs-129 | 1E-05 | 2E-06 | 9E+4 | 2E+4 | 3E+4 |
| Cs-130 ³⁸ | 8E-05 | 1E-05 | 6E+5 | 6E+4 | 2E+5 |
| Cs-131 | 1E-05 | 7E-06 | 2E+5 | 2E+4 | 3E+4 |
| Cs-132 | 2E-06 | 9E-07 | 3E+4 | 3E+3 | 4E+3 |
| Cs-134m | 6E-05 | 8E-06 | 2E+5 | 1E+5 | 1E+5 |
| Cs-134 | 4E-08 | 5E-08 | 2E+3 | 70 | 1E+2 |
| Cs-135m ³⁸ | 8E-05 | 8E-06 | 2E+5 | 1E+5 | 2E+5 |
| Cs-135 | 5E-07 | 5E-07 | 2E+4 | 7E+2 | 1E+3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|----------------------|-------------------------------------|--------------------------------------|-------------------------|----------------------------------|
| | | | | Ingestion Inhalation |
| Cs-136 | 3E-07 | 2E-07 | 1E+4 | 4E+2 7E+2 |
| Cs-137 | 6E-08 | 8E-08 | 3E+3 | 1E+2 2E+2 |
| Cs-138 ³⁸ | 2E-05 | 5E-06 | 2E+5 | 2E+4 6E+4 |
| Ba-126 ³⁸ | 6E-06 | 4E-06 | 1E+5 | 6E+3 2E+4 |
| Ba-128 | 7E-07 | 4E-07 | 1E+4 | 5E+2 2E+3 |
| Ba-131m | 6E-04 | 4E-05 | 1E+6 | 4E+5 1E+6 |
| Ba-131 | 3E-06 | 1E-06 | 4E+4 | 3E+3 8E+3 |
| Ba-133m | 4E-06 | 2E-06 | 7E+4 | 2E+3 9E+3 |
| Ba-133 | 3E-07 | 3E-07 | 1E+4 | 2E+3 7E+2 |
| Ba-135m | 5E-06 | 2E-06 | 9E+4 | 3E+3 1E+4 |
| Ba-139 ³⁸ | 1E-05 | 1E-05 | 3E+5 | 1E+4 3E+4 |
| Ba-140 | 6E-07 | 3E-07 | 1E+4 | 5E+2 1E+3 |
| Ba-141 ³⁸ | 3E-05 | 1E-05 | 4E+5 | 2E+4 7E+4 |
| Ba-142 ³⁸ | 6E-05 | 9E-06 | 3E+5 | 5E+4 1E+5 |
| La-131 ³⁸ | 5E-05 | 8E-06 | 3E+5 | 5E+4 1E+5 |
| La-132 | 4E-06 | 1E-06 | 5E+4 | 3E+3 1E+4 |
| La-135 | 4E-05 | 1E-05 | 4E+5 | 4E+4 9E+4 |
| La-137 | 3E-08 | 4E-08 | 1E+3 | 1E+4 60 |
| La-138 | 1E-09 | 3E-09 | 1E+2 | 9E+2 4 |
| La-140 | 5E-07 | 3E-07 | 1E+4 | 6E+2 1E+3 |
| La-141 | 4E-06 | 2E-06 | 9E+4 | 4E+3 9E+3 |
| La-142 ³⁸ | 9E-06 | 2E-06 | 8E+4 | 8E+3 2E+4 |
| La-143 ³⁸ | 4E-05 | 1E-05 | 4E+5 | 4E+4 9E+4 |
| Ce-134 | 3E-07 | 3E-07 | 1E+4 | 5E+2 7E+2 |
| Ce-135 | 2E-06 | 5E-07 | 2E+4 | 2E+3 4E+3 |
| Ce-137m | 2E-06 | 9E-07 | 3E+4 | 2E+3 4E+3 |
| Ce-137 | 5E-05 | 1E-05 | 7E+5 | 5E+4 1E+5 |
| Ce-139 | 3E-07 | 4E-07 | 1E+4 | 5E+3 7E+2 |
| Ce-141 | 2E-07 | 1E-07 | 6E+3 | 2E+3 6E+2 |
| Ce-143 | 7E-07 | 5E-07 | 2E+4 | 1E+3 2E+3 |

| | 10CFR20 DAC µCi/mL | 10CFR835 DAC µCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|------------------------------------|
| | | | | Ingestion Inhalation |
| Ce-144 | 6E-09 | 1E-08 | 7E+2 | 2E+2 10 |
| Pr-136 ³⁸ | 9E-05 | 1E-05 | 3E+5 | 5E+4 2E+5 |
| Pr-137 ³⁸ | 6E-05 | 9E-06 | 3E+5 | 4E+4 1E+5 |
| Pr-138m | 2E-05 | 2E-06 | 7E+4 | 1E+4 4E+4 |
| Pr-139 | 5E-05 | 1E-05 | 2E+5 | 4E+4 1E+5 |
| Pr-142m ³⁸ | 6E-05 | 5E-05 | 2E+6 | 8E+4 1E+5 |
| Pr-142 | 8E-07 | 7E-07 | 2E+4 | 1E+3 2E+3 |
| Pr-143 | 3E-07 | 2E-07 | 9E+3 | 9E+2 7E+2 |
| Pr-144 ³⁸ | 5E-05 | 1E-05 | 4E+5 | 3E+4 1E+5 |
| Pr-145 | 3E-06 | 2E-06 | 8E+4 | 3E+3 8E+3 |
| Pr-147 ³⁸ | 8E-05 | 9E-06 | 3E+5 | 5E+4 2E+5 |
| Nd-136 ³⁸ | 2E-05 | 4E-06 | 1E+5 | 1E+4 5E+4 |
| Nd-138 | 2E-06 | 1E-06 | 5E+4 | 2E+3 5E+3 |
| Nd-139m | 6E-06 | 1E-06 | 5E+4 | 5E+3 1E+4 |
| Nd-139 ³⁸ | 1E-04 | 1E-05 | 6E+5 | 9E+4 3E+5 |
| Nd-141 | 3E-04 | 3E-05 | 1E+6 | 2E+5 6E+5 |
| Nd-147 | 4E-07 | 2E-07 | 9E+3 | 1E+3 8E+2 |
| Nd-149 ³⁸ | 1E-05 | 4E-06 | 1E+5 | 1E+4 2E+4 |
| Nd-151 ³⁸ | 8E-05 | 9E-06 | 3E+5 | 7E+4 2E+5 |
| Pm-141 ³⁸ | 7E-05 | 1E-05 | 4E+5 | 5E+4 2E+5 |
| Pm-143 | 2E-07 | 5E-07 | 2E+4 | 5E+3 6E+2 |
| Pm-144 | 5E-08 | 1E-07 | 3E+3 | 1E+3 1E+2 |
| Pm-145 | 7E-08 | 1E-07 | 1E+4 | 1E+4 2E+2 |
| Pm-146 | 2E-08 | 4E-08 | 1E+3 | 2E+3 40 |
| Pm-147 | 5E-08 | 1E-07 | 4E+3 | 4E+3 1E+2 |
| Pm-148m | 1E-07 | 1E-07 | 4E+3 | 7E+2 3E+2 |
| Pm-148 | 2E-07 | 2E-07 | 9E+3 | 4E+2 5E+2 |
| Pm-149 | 8E-07 | 6E-07 | 2E+4 | 1E+3 2E+3 |
| Pm-150 | 7E-06 | 2E-06 | 8E+4 | 5E+3 2E+4 |
| Pm-151 | 1E-06 | 8E-07 | 3E+4 | 2E+3 3E+3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| Sm-141m ³⁸ | 4E-05 | 5E-06 | 2E+5 | 3E+4 | 1E+5 |
| Sm-141 ³⁸ | 8E-05 | 1E-05 | 4E+5 | 5E+4 | 2E+5 |
| Sm-142 ³⁸ | 1E-05 | 4E-06 | 1E+5 | 8E+3 | 3E+4 |
| Sm-145 | 2E-07 | 4E-07 | 1E+4 | 6E+3 | 5E+2 |
| Sm-146 | 1E-11 | 2E-11 | 1 | 10 | 4E-2 |
| Sm-147 | 2E-11 | 2E-11 | 1 | 20 | 4E-2 |
| Sm-151 | 4E-08 | 7E-08 | 2E+3 | 1E+4 | 1E+2 |
| Sm-153 | 1E-06 | 8E-07 | 3E+4 | 2E+3 | 3E+3 |
| Sm-155 ³⁸ | 9E-05 | 1E-05 | 3E+5 | 6E+4 | 2E+5 |
| Sm-156 | 4E-06 | 2E-06 | 7E+4 | 5E+3 | 9E+3 |
| Eu-145 | 8E-07 | 5E-07 | 2E+4 | 2E+3 | 2E+3 |
| Eu-146 | 5E-07 | 3E-07 | 1E+4 | 1E+3 | 1E+3 |
| Eu-147 | 7E-07 | 5E-07 | 2E+4 | 3E+3 | 2E+3 |
| Eu-148 | 1E-07 | 2E-07 | 9E+3 | 1E+3 | 4E+2 |
| Eu-149 | 1E-06 | 2E-06 | 9E+4 | 1E+4 | 3E+3 |
| Eu-150 ²² | 4E-06 | 2E-06 | 7E+4 | 3E+3 | 8E+3 |
| Eu-150 ²³ | 8E-09 | 1E-08 | 6E+2 | 8E+2 | 20 |
| Eu-152m | 3E-06 | 1E-06 | 6E+4 | 3E+3 | 6E+3 |
| Eu-152 | 1E-08 | 2E-08 | 7E+2 | 8E+2 | 20 |
| Eu-154 | 8E-09 | 1E-08 | 5E+2 | 5E+2 | 20 |
| Eu-155 | 4E-08 | 7E-08 | 2E+3 | 4E+3 | 90 |
| Eu-156 | 2E-07 | 1E-07 | 6E+3 | 6E+2 | 5E+2 |
| Eu-157 | 2E-06 | 1E-06 | 4E+4 | 2E+3 | 5E+3 |
| Eu-158 ³⁸ | 2E-05 | 5E-06 | 1E+5 | 2E+4 | 6E+4 |
| Gd-145 ³⁸ | 6E-05 | 7E-06 | 2E+5 | 5E+4 | 2E+5 |
| Gd-146 | 5E-08 | 1E-07 | 4E+3 | 1E+3 | 1E+2 |
| Gd-147 | 1E-06 | 6E-07 | 2E+4 | 2E+3 | 4E+3 |
| Gd-148 | 3E-12 | 5E-12 | 0.2 | 10 | 8E-3 |
| Gd-149 | 9E-07 | 7E-07 | 2E+4 | 3E+3 | 2E+3 |
| Gd-151 | 2E-07 | 2E-07 | 9E+3 | 6E+3 | 4E+2 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|------------------------------------|
| | | | | Ingestion Inhalation |
| Gd-152 | 4E-12 | 7E-12 | 0.2 | 20 1E-2 |
| Gd-153 | 6E-08 | 9E-08 | 3E+3 | 5E+3 1E+2 |
| Gd-159 | 2E-06 | 1E-06 | 5E+4 | 3E+3 6E+3 |
| Tb-147 ³⁸ | 1E-05 | 2E-06 | 1E+5 | 9E+3 3E+4 |
| Tb-149 | 3E-07 | 1E-07 | 6E+3 | 5E+3 7E+2 |
| Tb-150 | 9E-06 | 2E-06 | 8E+4 | 5E+3 2E+4 |
| Tb-151 | 4E-06 | 1E-06 | 4E+4 | 4E+3 9E+3 |
| Tb-153 | 3E-06 | 2E-06 | 8E+4 | 5E+3 7E+3 |
| Tb-154 | 2E-06 | 5E-07 | 2E+4 | 2E+3 4E+3 |
| Tb-155 | 3E-06 | 2E-06 | 8E+4 | 6E+3 8E+3 |
| Tb-156m ²⁴ | 3E-06 | 2E-06 | 9E+4 | 2E+4 3E+4 |
| Tb-156m ²⁵ | 1E-05 | 4E-06 | 1E+5 | 7E+3 8E+3 |
| Tb-156 | 6E-07 | 4E-07 | 1E+4 | 1E+3 1E+3 |
| Tb-157 | 1E-07 | 2E-07 | 8E+3 | 5E+4 3E+2 |
| Tb-158 | 8E-09 | 1E-08 | 6E+2 | 1E+3 20 |
| Tb-160 | 9E-08 | 1E-07 | 3E+3 | 7E+2 2E+2 |
| Tb-161 | 7E-07 | 4E-07 | 1E+4 | 2E+3 2E+3 |
| Dy-155 | 1E-05 | 2E-06 | 1E+5 | 9E+3 3E+4 |
| Dy-157 | 3E-05 | 5E-06 | 1E+5 | 2E+4 6E+4 |
| Dy-159 | 1E-06 | 2E-06 | 8E+4 | 1E+4 2E+3 |
| Dy-165 | 2E-05 | 6E-06 | 2E+5 | 1E+4 5E+4 |
| Dy-166 | 3E-07 | 3E-07 | 1E+4 | 6E+2 7E+2 |
| Ho-155 ³⁸ | 6E-05 | 1E-05 | 4E+5 | 4E+4 2E+5 |
| Ho-157 ³⁸ | 6E-04 | 2E-05 | 1E+6 | 3E+5 1E+6 |
| Ho-159 ³⁸ | 4E-04 | 2E-05 | 9E+5 | 2E+5 1E+6 |
| Ho-161 | 2E-04 | 3E-05 | 1E+6 | 1E+5 4E+5 |
| Ho-162m ³⁸ | 1E-04 | 9E-06 | 3E+5 | 5E+4 3E+5 |
| Ho-162 ³⁸ | 1E-03 | 5E-05 | 2E+6 | 5E+5 2E+6 |
| Ho-164m ³⁸ | 1E-04 | 3E-05 | 1E+6 | 1E+5 3E+5 |
| Ho-164 ³⁸ | 3E-04 | 2E-05 | 8E+5 | 2E+5 6E+5 |

| | 10CFR20 DAC | μCi/mL | 10CFR835 DAC | μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | Ingestion | Inhalation |
|----------------------|--------------------|---------------|---------------------|---------------|-------------------------|-------------------------|------------------|-------------------|
| Ho-166m | 3E-09 | | 7E-09 | 2E+2 | | 6E+2 | | 70 |
| Ho-166 | 7E-07 | | 6E-07 | 2E+4 | | 9E+2 | | 2E+3 |
| Ho-167 | 2E-05 | | 4E-06 | 1E+5 | | 2E+4 | | 6E+4 |
| Er-161 | 3E-05 | | 3E-06 | 1E+5 | | 2E+4 | | 6E+4 |
| Er-165 | 8E-05 | | 2E-05 | 1E+6 | | 6E+4 | | 2E+5 |
| Er-169 | 1E-06 | | 6E-07 | 2E+4 | | 3E+3 | | 3E+3 |
| Er-171 | 4E-06 | | 1E-06 | 6E+4 | | 4E+3 | | 1E+4 |
| Er-172 | 6E-07 | | 4E-07 | 1E+4 | | 1E+3 | | 1E+3 |
| Tm-162 ³⁸ | 1E-04 | | 9E-06 | 3E+5 | | 7E+4 | | 3E+5 |
| Tm-166 | 6E-06 | | 1E-06 | 4E+4 | | 4E+3 | | 1E+4 |
| Tm-167 | 8E-07 | | 5E-07 | 2E+4 | | 2E+3 | | 2E+3 |
| Tm-170 | 9E-08 | | 1E-07 | 4E+3 | | 8E+2 | | 2E+2 |
| Tm-171 | 1E-07 | | 2E-07 | 9E+3 | | 1E+4 | | 3E+2 |
| Tm-172 | 5E-07 | | 4E-07 | 1E+4 | | 7E+2 | | 1E+3 |
| Tm-173 | 5E-06 | | 2E-06 | 8E+4 | | 4E+3 | | 1E+4 |
| Tm-175 ³⁸ | 1E-04 | | 8E-06 | 2E+5 | | 7E+4 | | 3E+5 |
| Yb-162 ³⁸ | 1E-04 | | 1E-05 | 5E+5 | | 7E+4 | | 3E+5 |
| Yb-166 | 8E-07 | | 5E-07 | 2E+4 | | 1E+3 | | 3E+3 |
| Yb-167 ³⁸ | 3E-04 | | 3E-05 | 1E+6 | | 3E+5 | | 7E+5 |
| Yb-169 | 3E-07 | | 2E-07 | 8E+3 | | 2E+3 | | 7E+2 |
| Yb-175 | 1E-06 | | 8E-07 | 2E+4 | | 3E+3 | | 3E+3 |
| Yb-177 ³⁸ | 2E-05 | | 5E-06 | 2E+5 | | 2E+4 | | 5E+4 |
| Yb-178 ³⁸ | 2E-05 | | 5E-06 | 1E+5 | | 1E+4 | | 4E+4 |
| Lu-169 | 2E-06 | | 9E-07 | 3E+4 | | 3E+3 | | 4E+3 |
| Lu-170 | 8E-07 | | 4E-07 | 1E+4 | | 1E+3 | | 2E+3 |
| Lu-171 | 8E-07 | | 6E-07 | 2E+4 | | 2E+3 | | 2E+3 |
| Lu-172 | 5E-07 | | 3E-07 | 1E+4 | | 1E+3 | | 1E+3 |
| Lu-173 | 1E-07 | | 2E-07 | 8E+3 | | 5E+3 | | 3E+2 |
| Lu-174m | 9E-08 | | 2E-07 | 7E+3 | | 2E+3 | | 2E+2 |
| Lu-174 | 5E-08 | | 9E-08 | 3E+3 | | 5E+3 | | 1E+2 |

| | 10CFR20 DAC | 10CFR835 DAC | 10CFR20 ALIs uCi |
|-----------------------|--------------------|--------------------------------|-----------------------------|
| | μCi/mL | μCi/mL Bq/M³ | Ingestion Inhalation |
| Lu-176m | 9E-06 | 3E-06 | 1E+5 8E+3 2E+4 |
| Lu-176 | 2E-09 | 3E-09 | 1E+2 7E+2 50 |
| Lu-177m | 3E-08 | 4E-08 | 1E+3 7E+2 80 |
| Lu-177 | 9E-07 | 5E-07 | 1E+4 2E+3 2E+3 |
| Lu-178m ³⁸ | 7E-05 | 4E-06 | 1E+5 5E+4 2E+5 |
| Lu-178 | 5E-05 | 8E-06 | 3E+5 4E+4 1E+5 |
| Lu-179 | 6E-06 | 3E-06 | 1E+5 6E+3 2E+4 |
| Hf-170 | 2E-06 | 1E-06 | 4E+4 3E+3 5E+3 |
| Hf-172 | 4E-09 | 6E-09 | 2E+2 1E+3 90 |
| Hf-173 | 5E-06 | 2E-06 | 8E+4 5E+3 1E+4 |
| Hf-175 | 4E-07 | 5E-07 | 2E+4 3E+3 9E+2 |
| Hf-177m ³⁸ | 2E-05 | 1E-06 | 6E+4 2E+4 6E+4 |
| Hf-178m | 5E-10 | 8E-10 | 30 3E+2 10 |
| Hf-179m | 1E-07 | 1E-07 | 6E+3 1E+3 3E+2 |
| Hf-180m | 9E-06 | 1E-06 | 6E+4 7E+3 2E+4 |
| Hf-181 | 7E-08 | 1E-07 | 4E+3 1E+3 2E+2 |
| Hf-182m ³⁸ | 4E-05 | 4E-06 | 1E+5 4E+4 9E+4 |
| Hf-182 | 3E-10 | 5E-10 | 20 2E+2 0.8 |
| Hf-183 ³⁸ | 2E-05 | 4E-06 | 1E+5 2E+4 5E+4 |
| Hf-184 | 3E-06 | 1E-06 | 4E+4 2E+3 6E+3 |
| Ta-172 ³⁸ | 4E-05 | 5E-06 | 1E+5 4E+4 1E+5 |
| Ta-173 | 7E-06 | 3E-06 | 1E+5 7E+3 2E+4 |
| Ta-174 ³⁸ | 4E-05 | 5E-06 | 2E+5 3E+4 9E+4 |
| Ta-175 | 6E-06 | 1E-06 | 6E+4 6E+3 1E+4 |
| Ta-176 | 5E-06 | 1E-06 | 3E+4 4E+3 1E+4 |
| Ta-177 | 7E-06 | 4E-06 | 1E+5 1E+4 2E+4 |
| Ta-178 | 3E-05 | 3E-06 | 1E+5 2E+4 7E+4 |
| Ta-179 | 4E-07 | 1E-06 | 7E+4 2E+4 9E+2 |
| Ta-180m | 2E-05 | 9E-06 | 3E+5 2E+4 6E+4 |
| Ta-180 | 1E-08 | 4E-08 | 1E+3 1E+3 20 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| Ta-182m ³⁸ | 2E-04 | 6E-06 | 2E+5 | 2E+5 | 4E+5 |
| Ta-182 | 6E-08 | 7E-08 | 2E+3 | 8E+2 | 1E+2 |
| Ta-183 | 4E-07 | 2E-07 | 1E+4 | 9E+2 | 1E+3 |
| Ta-184 | 2E-06 | 8E-07 | 3E+4 | 2E+3 | 5E+3 |
| Ta-185 ³⁸ | 3E-05 | 5E-06 | 1E+5 | 3E+4 | 6E+4 |
| Ta-186 ³⁸ | 9E-05 | 7E-06 | 2E+5 | 5E+4 | 2E+5 |
| W-176 | 2E-05 | 3E-06 | 1E+5 | 1E+4 | 5E+4 |
| W-177 | 4E-05 | 5E-06 | 2E+5 | 2E+4 | 9E+4 |
| W-178 | 8E-06 | 3E-06 | 1E+5 | 5E+3 | 2E+4 |
| W-179 ³⁸ | 7E-04 | 1E-04 | 5E+6 | 5E+5 | 2E+6 |
| W-181 | 1E-05 | 1E-05 | 4E+5 | 2E+4 | 3E+4 |
| W-185 | 3E-06 | 2E-06 | 9E+4 | 2E+3 | 7E+3 |
| W-187 | 4E-06 | 1E-06 | 5E+4 | 2E+3 | 9E+3 |
| W-188 | 5E-07 | 6E-07 | 2E+4 | 4E+2 | 2E+3 |
| Re-177 ³⁸ | 1E-04 | 1E-05 | 4E+5 | 9E+4 | 3E+5 |
| Re-178 ³⁸ | 1E-04 | 1E-05 | 3E+5 | 7E+4 | 3E+5 |
| Re-181 | 4E-06 | 1E-06 | 4E+4 | 5E+3 | 8E+3 |
| Re-182 ²⁶ | 9E-07 | 3E-07 | 1E+4 | 1E+3 | 1E+4 |
| Re-182 ²⁷ | 5E-06 | 1E-06 | 4E+4 | 1E+3 | 2E+3 |
| Re-184m | 2E-07 | 1E-07 | 4E+3 | 2E+3 | 4E+2 |
| Re-184 | 6E-07 | 3E-07 | 1E+4 | 2E+3 | 2E+3 |
| Re-186m | 6E-08 | 7E-08 | 2E+3 | 1E+3 | 2E+2 |
| Re-186 | 7E-07 | 4E-07 | 1E+4 | 2E+3 | 2E+3 |
| Re-187 | 4E-05 | 1E-04 | 4E+6 | 6E+5 | 1E+5 |
| Re-188m | 6E-05 | 2E-05 | 1E+6 | 8E+4 | 1E+5 |
| Re-188 | 2E-06 | 7E-07 | 2E+4 | 2E+3 | 3E+3 |
| Re-189 | 2E-06 | 9E-07 | 3E+4 | 3E+3 | 4E+3 |
| Os-180 ³⁸ | 2E-04 | 1E-05 | 3E+5 | 1E+5 | 4E+5 |
| Os-181 ³⁸ | 2E-05 | 3E-06 | 1E+5 | 1E+4 | 4E+4 |
| Os-182 | 2E-06 | 9E-07 | 3E+4 | 2E+3 | 4E+3 |

| | 10CFR20 DAC µCi/mL | 10CFR835 DAC µCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|------------------------------------|
| | | | | Ingestion Inhalation |
| Os-185 | 2E-07 | 4E-07 | 1E+4 | 2E+3 5E+2 |
| Os-189m | 7E-05 | 7E-05 | 2E+6 | 8E+4 2E+5 |
| Os-191m | 7E-06 | 4E-06 | 1E+5 | 1E+4 2E+4 |
| Os-191 | 6E-07 | 3E-07 | 1E+4 | 2E+3 1E+3 |
| Os-193 | 1E-06 | 8E-07 | 3E+4 | 2E+3 3E+3 |
| Os-194 | 3E-09 | 1E-08 | 4E+2 | 4E+2 8 |
| Ir-182 ³⁸ | 5E-05 | 7E-06 | 2E+5 | 4E+4 1E+5 |
| Ir-184 | 1E-05 | 1E-06 | 6E+4 | 8E+3 2E+4 |
| Ir-185 | 4E-06 | 1E-06 | 7E+4 | 5E+3 1E+4 |
| Ir-186 ²⁸ | X | 7E-07 | 2E+4 | X X |
| Ir-186 ²⁹ | X | 4E-06 | 1E+5 | X X |
| Ir-186 | 2E-06 | X | X | 2E+3 6E+3 |
| Ir-187 | 1E-05 | 3E-06 | 1E+5 | 1E+4 3E+4 |
| Ir-188 | 1E-06 | 6E-07 | 2E+4 | 2E+3 3E+3 |
| Ir-189 | 1E-06 | 1E-06 | 4E+4 | 5E+3 4E+3 |
| Ir-190m ³⁸ | 8E-05 | X | X | 2E+5 2E+5 |
| Ir-190m ³⁰ | X | 2E-06 | 7E+4 | X X |
| Ir-190m ³¹ | X | 5E-05 | 1E+6 | X X |
| Ir-190 | 4E-07 | 2E-07 | 8E+3 | 1E+3 9E+2 |
| Ir-192m | 6E-09 | 1E-07 | 1E+3 | 3E+3 90 |
| Ir-192 | 9E-08 | 1E-07 | 4E+3 | 3E+2 2E+2 |
| Ir-194m | 3E-08 | 8E-08 | 2E+3 | 6E+2 90 |
| Ir-194 | 8E-07 | 7E-07 | 2E+4 | 1E+3 2E+3 |
| Ir-195m | 9E-06 | 2E-06 | 7E+4 | 8E+2 2E+4 |
| Ir-195 | 2E-05 | 4E-06 | 1E+5 | 1E+4 4E+4 |
| Pt-186 | 2E-05 | 3E-06 | 1E+5 | 1E+4 4E+4 |
| Pt-188 | 7E-07 | 8E-07 | 3E+4 | 2E+3 2E+3 |
| Pt-189 | 1E-05 | 3E-06 | 1E+5 | 1E+4 3E+4 |
| Pt-191 | 4E-06 | 1E-06 | 7E+4 | 4E+3 8E+3 |
| Pt-193m | 3E-06 | 2E-06 | 8E+4 | 3E+3 6E+3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|----------------------------------|
| | | | | Ingestion Inhalation |
| Pt-193 | 1E-05 | 2E-05 | 7E+5 | 4E+4 2E+4 |
| Pt-195m | 2E-06 | 1E-06 | 5E+4 | 2E+3 4E+3 |
| Pt-197m ³⁸ | 2E-05 | 7E-06 | 2E+5 | 2E+4 4E+4 |
| Pt-197 | 4E-06 | 3E-06 | 1E+5 | 3E+3 1E+4 |
| Pt-199 ³⁸ | 6E-05 | 1E-05 | 4E+5 | 5E+4 1E+5 |
| Pt-200 | 1E-06 | 1E-06 | 5E+4 | 1E+3 3E+3 |
| Au-193 | 8E-06 | 3E-06 | 1E+5 | 9E+3 2E+4 |
| Au-194 | 2E-06 | 9E-07 | 3E+4 | 3E+3 5E+3 |
| Au-195 | 2E-07 | 4E-07 | 1E+4 | 5E+3 4E+2 |
| Au-198m | 5E-07 | 2E-07 | 1E+4 | 1E+3 1E+3 |
| Au-198 | 7E-07 | 5E-07 | 1E+4 | 1E+3 2E+3 |
| Au-199 | 2E-06 | 7E-07 | 2E+4 | 3E+3 4E+3 |
| Au-200m | 1E-06 | 4E-07 | 1E+4 | 1E+3 3E+3 |
| Au-200 | 3E-05 | 7E-06 | 2E+5 | 3E+4 6E+4 |
| Au-201 | 9E-05 | 9E-06 | 3E+5 | 7E+4 2E+5 |
| Hg-193m ³² | 5E-06 | 1E-06 | 4E+4 | 4E+3 1E+4 |
| Hg-193m | 3E-06 | 1E-06 | 4E+4 | 3E+3 8E+3 |
| Hg-193m ¹⁰ | 4E-06 | 1E-07 | 6E+3 | X 8E+3 |
| Hg-193 ³² | 3E-05 | 5E-06 | 1E+5 | 2E+4 6E+4 |
| Hg-193 | 2E-05 | 4E-06 | 1E+5 | 2E+4 4E+4 |
| Hg-193 ¹⁰ | 1E-05 | 5E-07 | 1E+4 | X 3E+4 |
| Hg-194 ³² | 1E-08 | 2E-08 | 1E+3 | 20 30 |
| Hg-194 | 2E-05 | 3E-08 | 1E+3 | 8E+2 40 |
| Hg-194 ¹⁰ | 1E-08 | 1E-08 | 5E+2 | X 30 |
| Hg-195m ³² | 3E-06 | 1E-06 | 5E+4 | 3E+3 6E+3 |
| Hg-195m | 2E-06 | 8E-07 | 3E+4 | 2E+3 4E+3 |
| Hg-195m ¹⁰ | 2E-06 | 6E-08 | 2E+3 | X 4E+3 |
| Hg-195 ³² | 2E-05 | 6E-06 | 2E+5 | 2E+4 5E+4 |
| Hg-195 | 1E-05 | 6E-06 | 2E+5 | 1E+4 3E+4 |
| Hg-195 ¹⁰ | 1E-05 | 4E-07 | 1E+4 | X 3E+4 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| Hg-197m ³² | 4E-06 | 1E-06 | 5E+4 | 4E+3 | 9E+3 |
| Hg-197m | 2E-06 | 8E-07 | 3E+4 | 3E+3 | 5E+3 |
| Hg-197m ¹⁰ | 2E-06 | 9E-08 | 3E+3 | X | 5E+3 |
| Hg-197 ³² | 6E-06 | 4E-06 | 1E+5 | 7E+3 | 1E+4 |
| Hg-197 | 4E-06 | 2E-06 | 7E+4 | 6E+3 | 9E+3 |
| Hg-197 ¹⁰ | 4E-06 | 1E-07 | 4E+3 | X | 8E+3 |
| Hg-199m ³² | 7E-05 | 8E-06 | 3E+5 | 6E+4 | 2E+5 |
| Hg-199m ³⁸ | 6E-05 | 5E-06 | 1E+5 | 6E+4 | 1E+5 |
| Hg-199m ¹⁰ | 3E-05 | 3E-06 | 1E+5 | X | 8E+4 |
| Hg-203 ³² | 3E-07 | 7E-07 | 2E+4 | 5E+2 | 8E+2 |
| Hg-203 | 5E-07 | 2E-07 | 1E+4 | 2E+3 | 1E+3 |
| Hg-203 ¹⁰ | 4E-07 | 8E-08 | 2E+3 | X | 8E+2 |
| TI-194m ³⁸ | 6E-05 | 5E-06 | 2E+5 | 5E+4 | 2E+5 |
| TI-194 ³⁸ | 2E-04 | 2E-05 | 8E+5 | 3E+5 | 6E+5 |
| TI-195 ³⁸ | 5E-05 | 6E-06 | 2E+5 | 6E+4 | 1E+5 |
| TI-197 | 5E-05 | 8E-06 | 2E+5 | 7E+4 | 1E+5 |
| TI-198m ³⁸ | 2E-05 | 2E-06 | 9E+4 | 3E+4 | 5E+4 |
| TI-198 | 1E-05 | 1E-06 | 5E+4 | 2E+4 | 3E+4 |
| TI-199 | 4E-05 | 5E-06 | 2E+5 | 6E+4 | 8E+4 |
| TI-200 | 5E-06 | 8E-07 | 3E+4 | 8E+3 | 1E+4 |
| TI-201 | 9E-06 | 4E-06 | 1E+5 | 2E+4 | 2E+4 |
| TI-202 | 2E-06 | 1E-06 | 5E+4 | 4E+3 | 5E+3 |
| TI-204 | 9E-07 | 9E-07 | 3E+4 | 2E+3 | 2E+3 |
| Pb-195m ³⁸ | 8E-05 | 7E-06 | 2E+5 | 6E+4 | 2E+5 |
| Pb-198 | 3E-05 | 2E-06 | 9E+4 | 3E+4 | 6E+4 |
| Pb-199 ³⁸ | 3E-05 | 4E-06 | 1E+5 | 2E+4 | 7E+4 |
| Pb-200 | 3E-06 | 1E-06 | 4E+4 | 3E+3 | 6E+3 |
| Pb-201 | 8E-06 | 2E-06 | 7E+4 | 7E+3 | 2E+4 |
| Pb-202m | 1E-05 | 1E-06 | 6E+4 | 9E+3 | 3E+4 |
| Pb-202 | 2E-08 | 4E-08 | 1E+3 | 1E+2 | 50 |

| | 10CFR20 DAC µCi/mL | 10CFR835 DAC | | 10CFR20 ALIs uCi | |
|----------------------|-------------------------------------|---------------------|-------------------------|-------------------------|-------------------|
| | | µCi/mL | Bq/M³ | Ingestion | Inhalation |
| Pb-203 | 4E-06 | 2E-06 | 7E+4 | 5E+3 | 9E+3 |
| Pb-205 | 6E-07 | 9E-07 | 3E+4 | 4E+3 | 1E+3 |
| Pb-209 | 2E-05 | 9E-06 | 3E+5 | 2E+4 | 6E+4 |
| Pb-210 | 1E-10 | 1E-10 | 5 | 0.6 | 0.2 |
| Pb-211 ³⁸ | 3E-07 | 4E-08 | 1E+3 | 1E+4 | 6E+2 |
| Pb-212 | 2E-08 | 5E-09 | 2E+2 | 80 | 30 |
| Pb-214 ³⁸ | 3E-07 | 4E-08 | 1E+3 | 9E+3 | 8E+2 |
| Bi-200 ³⁸ | 4E-05 | 4E-06 | 1E+5 | 3E+4 | 8E+4 |
| Bi-201 ³⁸ | 1E-05 | 2E-06 | 1E+5 | 1E+4 | 3E+4 |
| Bi-202 ³⁸ | 2E-05 | 2E-06 | 9E+4 | 1E+4 | 4E+4 |
| Bi-203 | 3E-06 | 7E-07 | 2E+4 | 2E+3 | 6E+3 |
| Bi-205 | 5E-07 | 4E-07 | 1E+4 | 1E+3 | 1E+3 |
| Bi-206 | 4E-07 | 2E-07 | 8E+3 | 6E+2 | 9E+2 |
| Bi-207 | 1E-07 | 1E-07 | 6E+3 | 1E+3 | 4E+2 |
| Bi-210m | 3E-10 | 2E-10 | 9 | 40 | 0.7 |
| Bi-210 | 1E-08 | 9E-09 | 3E+2 | 8E+2 | 30 |
| Bi-212 ³⁸ | 1E-07 | 8E-09 | 3E+2 | 5E+3 | 2E+2 |
| Bi-213 ³⁸ | 1E-07 | 7E-09 | 2E+2 | 7E+3 | 3E+2 |
| Bi-214 ³⁸ | 3E-07 | 1E-08 | 4E+2 | 2E+4 | 8E+2 |
| Po-203 ³⁸ | 3E-05 | 4E-06 | 1E+5 | 3E+4 | 6E+4 |
| Po-205 ³⁸ | 2E-05 | 3E-06 | 1E+5 | 2E+4 | 4E+4 |
| Po-207 | 1E-05 | 1E-06 | 6E+4 | 8E+3 | 3E+4 |
| Po-210 | 3E-10 | 2E-10 | 9 | 3 | 0.6 |
| At-207 ³⁸ | 2E-08 | 2E-07 | 1E+4 | 6E+3 | 2E+3 |
| At-211 | 2E-08 | 5E-09 | 1E+2 | 1E+2 | 50 |
| Rn-220 ³³ | X | 1E-08 | 6E+2 | X | X |
| Rn-220 ³⁴ | 7E-06 | X | X | X | 2E+4 |
| Rn-220 ³⁵ | 9E-09 | X | X | X | 20 |
| Rn-222 ³³ | X | 8E-08 | 3E+3 | X | X |
| Rn-222 ³⁴ | 4E-06 | X | X | X | 1E+4 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL Bq/M³ | 10CFR20 ALIs uCi | |
|----------------------|-------------------------------------|---|-------------------------|-------------------|
| | | | Ingestion | Inhalation |
| Rn-222 ³⁵ | 3E-08 | X | X | X 1E+2 |
| Fr-222 ³⁸ | 2E-07 | 1E-08 | 3E+2 | 2E+3 5E+2 |
| Fr-223 ³⁸ | 3E-07 | 4E-07 | 1E+4 | 6E+2 8E+2 |
| Ra-223 | 3E-10 | 9E-11 | 3 | 50 0.7 |
| Ra-224 | 7E-10 | 2E-10 | 8 | 8 2 |
| Ra-225 | 3E-10 | 1E-10 | 4 | 8 0.7 |
| Ra-226 | 3E-10 | 2E-10 | 9 | 2 0.6 |
| Ra-227 ³⁸ | 6E-06 | 8E-07 | 3E+4 | 2E+4 1E+4 |
| Ra-228 | 5E-10 | 1E-10 | 5 | 2 1 |
| Ac-224 | 1E-08 | 5E-09 | 2E+2 | 2E+3 30 |
| Ac-225 | 1E-10 | 8E-11 | 3 | 50 0.3 |
| Ac-226 | 1E-09 | 5E-10 | 20 | 1E+2 3 |
| Ac-227 | 2E-13 | 2E-13 | 1E-2 | 0.2 4E-4 |
| Ac-228 | 4E-09 | 6E-09 | 2E+2 | 2E+3 9 |
| Th-226 ³⁸ | 6E-08 | 4E-09 | 1E+2 | 5E+3 1E+2 |
| Th-227 | 1E-10 | 7E-11 | 2 | 1E+2 0.3 |
| Th-228 | 4E-12 | 2E-11 | 0.7 | 6 1E-2 |
| Th-229 | 4E-13 | 2E-12 | 7E-2 | 0.6 9E-4 |
| Th-230 | 3E-12 | 3E-12 | 0.1 | 4 6E-3 |
| Th-231 | 3E-06 | 1E-06 | 5E+4 | 4E+3 6E+3 |
| Th-232 | 5E-13 | 3E-12 | 0.1 | 0.7 1E-3 |
| Th-234 | 6E-08 | 9E-08 | 3E+3 | 3E+2 2E+2 |
| Pa-227 ³⁸ | 4E-08 | 4E-09 | 1E+2 | 4E+3 1E+2 |
| Pa-228 | 5E-09 | 1E-08 | 3E+2 | 1E+3 10 |
| Pa-230 | 1E-09 | 9E-10 | 30 | 6E+2 40 |
| Pa-231 | 6E-13 | 1E-12 | 4E-2 | 0.2 2E-3 |
| Pa-232 | 9E-09 | 1E-08 | 6E+2 | 1E+3 20 |
| Pa-233 | 2E-07 | 1E-07 | 6E+3 | 1E+3 6E+2 |
| Pa-234 | 3E-06 | 7E-07 | 2E+4 | 2E+3 7E+3 |
| U-230 | 1E-10 | 4E-11 | 1 | 4 0.3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL Bq/M³ | | 10CFR20 ALIs uCi | |
|----------------------|-------------------------------------|---|------------|-------------------------|------|
| | | Ingestion | Inhalation | | |
| U-231 | 2E-06 | 1E-06 | 4E+4 | 4E+3 | 5E+3 |
| U-232 | 3E-12 | 2E-11 | 0.7 | 2 | 8E-3 |
| U-233 | 2E-11 | 7E-11 | 2 | 10 | 4E-2 |
| U-234 | 2E-11 | 7E-11 | 2 | 10 | 4E-2 |
| U-235 | 2E-11 | 8E-11 | 3 | 10 | 4E-2 |
| U-236 | 2E-11 | 7E-11 | 2 | 10 | 4E-2 |
| U-237 | 6E-07 | 3E-07 | 1E+4 | 2E+3 | 2E+3 |
| U-238 | 2E-11 | 8E-11 | 3 | 10 | 4E-2 |
| U-239 ³⁸ | 7E-05 | 9E-06 | 3E+5 | 7E+4 | 2E+5 |
| U-240 | 1E-06 | 6E-07 | 2E+4 | 1E+3 | 2E+3 |
| U-Natural | 2E-11 | X | X | 10 | 5E-2 |
| Np-232 ³⁸ | 7E-07 | 3E-06 | 1E+5 | 1E+5 | 5E+2 |
| Np-233 ³⁸ | 1E-03 | 7E-05 | 2E+6 | 8E+5 | 3E+6 |
| Np-234 | 1E-06 | 5E-07 | 2E+4 | 2E+3 | 3E+3 |
| Np-235 | 3E-07 | 1E-06 | 4E+4 | 2E+4 | 8E+2 |
| Np-236 ³⁶ | 9E-12 | 4E-11 | 1 | 3 | 5E-2 |
| Np-236 ³⁷ | 1E-08 | 5E-08 | 1E+3 | 3E+3 | 30 |
| Np-237 | 2E-12 | 8E-12 | 0.3 | 0.5 | 4E-3 |
| Np-238 | 3E-08 | 1E-07 | 4E+3 | 1E+3 | 60 |
| Np-239 | 9E-07 | 5E-07 | 1E+4 | 2E+3 | 2E+3 |
| Np-240 ³⁸ | 3E-05 | 2E-06 | 8E+4 | 2E+4 | 6E+4 |
| Pu-234 | 8E-08 | 3E-08 | 1E+3 | 8E+3 | 2E+2 |
| Pu-235 ³⁸ | 1E-03 | 8E-05 | 3E+6 | 9E+5 | 3E+6 |
| Pu-236 | 8E-12 | 1E-11 | 0.6 | 20 | 2E-2 |
| Pu-237 | 1E-06 | 1E-06 | 6E+4 | 1E+4 | 3E+3 |
| Pu-238 | 3E-12 | 6E-12 | 0.2 | 0.9 | 7E-3 |
| Pu-239 | 3E-12 | 5E-12 | 0.2 | 0.83 | 6E-3 |
| Pu-240 | 3E-12 | 5E-12 | 0.2 | 0.8 | 6E-3 |
| Pu-241 | 1E-10 | 2E-10 | 10 | 40 | 0.3 |
| Pu-242 | 3E-12 | 5E-12 | 0.2 | 0.8 | 7E-3 |

| | 10CFR20 DAC μCi/mL | 10CFR835 DAC μCi/mL | Bq/M³ | 10CFR20 ALIs uCi | |
|-----------------------|-------------------------------------|--------------------------------------|-------------------------|-------------------------|-------------------|
| | | | | Ingestion | Inhalation |
| Pu-243 | 2E-05 | 5E-06 | 1E+5 | 2E+4 | 4E+4 |
| Pu-244 | 3E-12 | 5E-12 | 0.2 | 0.8 | 7E-3 |
| Pu-245 | 2E-06 | 8E-07 | 3E+4 | 2E+3 | 4E+3 |
| Pu-246 | 1E-07 | 8E-08 | 3E+3 | 4E+2 | 3E+2 |
| Am-237 ³⁸ | 1E-04 | 8E-06 | 3E+5 | 8E+4 | 3E+5 |
| Am-238 ³⁸ | 1E-06 | 2E-06 | 9E+4 | 4E+4 | 3E+3 |
| Am-239 | 5E-06 | 1E-06 | 6E+4 | 5E+3 | 1E+4 |
| Am-240 | 1E-06 | 7E-07 | 2E+4 | 2E+3 | 3E+3 |
| Am-241 | 3E-12 | 5E-12 | 0.1 | 0.8 | 6E-3 |
| Am-242m | 3E-12 | 5E-12 | 0.1 | 0.8 | 6E-3 |
| Am-242 | 4E-08 | 4E-08 | 1E+3 | 4E+3 | 80 |
| Am-243 | 3E-12 | 5E-12 | 0.1 | 0.8 | 6E-3 |
| Am-244m ³⁸ | 2E-06 | 3E-06 | 1E+5 | 6E+4 | 4E+3 |
| Am-244 | 8E-08 | 1E-07 | 5E+3 | 3E+3 | 2E+2 |
| Am-245 | 3E-05 | 5E-06 | 2E+5 | 3E+4 | 8E+4 |
| Am-246m ³⁸ | 8E-05 | 6E-06 | 2E+5 | 5E+4 | 2E+5 |
| Am-246 ³⁸ | 4E-05 | 2E-06 | 9E+4 | 3E+4 | 1E+5 |
| Cm-238 | 5E-07 | 1E-07 | 4E+3 | 2E+4 | 1E+3 |
| Cm-240 | 2E-10 | 2E-10 | 7 | 60 | 0.6 |
| Cm-241 | 1E-08 | 2E-08 | 8E+2 | 1E+3 | 30 |
| Cm-242 | 1E-10 | 1E-10 | 5 | 30 | 0.3 |
| Cm-243 | 4E-12 | 7E-12 | 0.2 | 10 | 9E-3 |
| Cm-244 | 5E-12 | 9E-12 | 0.3 | 10 | 1E-2 |
| Cm-245 | 3E-12 | 5E-12 | 0.1 | 0.7 | 6E-3 |
| Cm-246 | 3E-12 | 5E-12 | 0.1 | 0.7 | 6E-3 |
| Cm-247 | 3E-12 | 5E-12 | 0.2 | 0.8 | 6E-3 |
| Cm-248 | 7E-13 | 1E-12 | 5E-2 | 0.2 | 2E-3 |
| Cm-249 ³⁸ | 7E-06 | 8E-06 | 3E+5 | 5E+4 | 2E+4 |
| Cm-250 | 1E-13 | 2E-13 | 8E-3 | 4E-2 | 3E-4 |
| Bk-245 | 5E-07 | 3E-07 | 1E+4 | 2E+3 | 1E+3 |

| | 10CFR20 DAC µCi/mL | 10CFR835 DAC | | 10CFR20 ALIs uCi | |
|----------------------|-------------------------------------|---------------------|-------------------------|-------------------------|-------------------|
| | | µCi/mL | Bq/M³ | Ingestion | Inhalation |
| Bk-246 | 1E-06 | 8E-07 | 3E+4 | 3E+3 | 3E+3 |
| Bk-247 | 2E-12 | 3E-12 | 0.1 | 0.5 | 4E-3 |
| Bk-249 | 7E-10 | 1E-09 | 50 | 2E+2 | 20 |
| Bk-250 | 1E-07 | 2E-07 | 9E+3 | 9E+3 | 3E+2 |
| Cf-244 ³⁸ | 2E-07 | 1E-08 | 5E+2 | 3E+4 | 6E+2 |
| Cf-246 | 4E-09 | 1E-09 | 50 | 4E+2 | 90 |
| Cf-248 | 3E-11 | 5E-11 | 2 | 80 | 6E-2 |
| Cf-249 | 2E-12 | 3E-12 | 0.1 | 0.5 | 4E-3 |
| Cf-250 | 4E-12 | 7E-12 | 0.2 | 10 | 9E-3 |
| Cf-251 | 2E-12 | 3E-12 | 0.1 | 0.5 | 4E-3 |
| Cf-252 | 8E-12 | 1E-11 | 0.6 | 20 | 2E-2 |
| Cf-253 | 7E-10 | 5E-10 | 20 | 2E+2 | 20 |
| Cf-254 | 7E-12 | 2E-11 | 0.8 | 20 | 2E-2 |
| Es-250 | 2E-07 | 4E-07 | 1E+4 | 4E+4 | 5E+2 |
| Es-251 | 4E-07 | 3E-07 | 1E+4 | 7E+3 | 9E+2 |
| Es-253 | 6E-10 | 2E-10 | 9 | 2E+2 | 10 |
| Es-254m | 4E-09 | 1E-09 | 50 | 3E+2 | 10 |
| Es-254 | 3E-11 | 6E-11 | 2 | 80 | 7E-2 |
| Fm-252 | 5E-09 | 2E-09 | 80 | 5E+2 | 10 |
| Fm-253 | 4E-09 | 1E-09 | 60 | 1E+3 | 10 |
| Fm-254 | 4E-08 | 6E-09 | 2E+2 | 3E+3 | 90 |
| Fm-255 | 9E-09 | 2E-09 | 80 | 5E+2 | 20 |
| Fm-257 | 7E-11 | 1E-10 | 4 | 20 | 0.2 |
| Md-257 | 4E-08 | 2E-08 | 1E+3 | 7E+3 | 80 |
| Md-258 | 1E-10 | 1E-10 | 4 | 30 | 0.2 |

External Exposure in a Cloud of Airborne Material

| | 10CFR835 | 10CFR20 |
|---------|-------------------|-----------------|
| | $\mu\text{Ci/mL}$ | Bq/M^3 |
| Ar-37 | 10 | 4E+10 |
| Ar-39 | 4E-04 | 1E+07 |
| Ar-41 | 1E-06 | 3E+04 |
| Kr-74 | 1E-06 | 4E+04 |
| Kr-76 | 3E-06 | 1E+05 |
| Kr-77 | 1E-06 | 5E+04 |
| Kr-79 | 5E-06 | 2E+05 |
| Kr-81 | 2E-04 | 9E+06 |
| Kr-83m | 2E-02 | 9E+08 |
| Kr-85 | 2E-04 | 9E+06 |
| Kr-85m | 9E-06 | 3E+05 |
| Kr-87 | 1E-06 | 5E+04 |
| Kr-88 | 6E-07 | 2E+04 |
| Xe-120 | 3E-06 | 1E+05 |
| Xe-121 | 7E-07 | 2E+04 |
| Xe-122 | 2E-05 | 1E+06 |
| Xe-123 | 2E-06 | 8E+04 |
| Xe-125 | 5E-06 | 2E+05 |
| Xe-127 | 5E-06 | 2E+05 |
| Xe-129m | 6E-05 | 2E+06 |
| Xe-131m | 1E-04 | 6E+06 |
| Xe-133 | 4E-05 | 1E+06 |
| Xe-133m | 4E-05 | 1E+06 |
| Xe-135 | 5E-06 | 2E+05 |
| Xe-135m | 3E-06 | 1E+05 |
| Xe-138 | 1E-06 | 4E+04 |

STCs = Special Tritium Compounds

| | | | | | |
|----|---|---------------------|----|---|--|
| 1 | = | Water (HTO) form | 21 | = | Methyl |
| 2 | = | Elemental (HT form) | 22 | = | 12 h half-life |
| 3 | = | water and elemental | 23 | = | 34 yr half-life |
| 4 | = | Insoluble | 24 | = | 24 h half-life |
| 5 | = | Soluble | 25 | = | 5 h half-life |
| 6 | = | Vapor form | 26 | = | 64 h half-life |
| 7 | = | As CO | 27 | = | 12 h half-life |
| 8 | = | As CO ₂ | 28 | = | 16 h half-life |
| 9 | = | compounds | 29 | = | 2 h half-life |
| 10 | = | Vapor | 30 | = | 3 h half-life |
| 11 | = | Inorganic | 31 | = | 1 h half-life |
| 12 | = | Carbonyl | 32 | = | Organic |
| 13 | = | 66 min half-life | 33 | = | radon-220/222 with short-lived progeny |
| 14 | = | 122 min half-life | 34 | = | with progeny removed |
| 15 | = | 69 min half-life | 35 | = | with progeny present |
| 16 | = | 5 h half-life | 36 | = | 1E+05 yr half-life |
| 17 | = | 16 min half-life | 37 | = | 22 h half-life |
| 18 | = | 6 d half-life | 38 | = | half-life less than 2 h |
| 19 | = | 9 h half-life | | | |
| 20 | = | 10 min half-life | | | |

For any radionuclide not listed in these tables with decay mode other than alpha emission or spontaneous fission and with radioactive half-life less than two hours, the DAC value shall be 6E-06 $\mu\text{Ci/mL}$ (2E+04 Bq/M³).

The DAC values listed for both 10CFR20 and 10CFR835 were truncated after being calculated from the appropriate ALI values. For 10CFR835 the ALI values were taken from ICRP 68.

Characteristic X-Rays (KeV) of the Elements

These characteristic x-rays originate in the shell of the atom and can be used to identify specific elements but not a specific isotope. These characteristic x-rays are emitted from the shell of the atom after sufficient energy in the form of thermal heat, laser, micro-waves, or other type of energy is directed into the atom shell.

| Z # | | K _α | K _β | L _α | L _β |
|-----|----|----------------|----------------|----------------|----------------|
| 89 | Ac | 90.89 | 102.85 | 12.65 | 15.71 |
| 47 | Ag | 22.16 | 24.94 | 2.98 | 3.15 |
| 13 | Al | 1.49 | 1.55 | X | X |
| 95 | Am | 106.35 | 120.16 | 14.62 | 18.83 |
| 18 | Ar | 2.96 | 3.19 | X | X |
| 33 | As | 10.54 | 11.73 | 1.28 | 1.32 |
| 85 | At | 81.53 | 92.32 | 11.42 | 13.87 |
| 79 | Au | 68.79 | 77.97 | 9.71 | 11.44 |
| 5 | B | 0.185 | X | X | X |
| 56 | Ba | 32.19 | 36.38 | 4.47 | 4.83 |
| 4 | Be | 0.110 | X | X | X |
| 83 | Bi | 77.10 | 87.34 | 10.84 | 13.02 |
| 97 | Bk | 111.90 | 126.36 | 15.31 | 19.97 |
| 35 | Br | 11.92 | 13.29 | 1.48 | 1.53 |
| 6 | C | 0.282 | X | X | X |
| 20 | Ca | 3.69 | 4.01 | 0.34 | X |
| 48 | Cd | 23.17 | 26.09 | 3.13 | 3.32 |
| 58 | Ce | 34.72 | 39.26 | 4.84 | 5.26 |
| 98 | Cf | 114.75 | 129.54 | 15.66 | 20.56 |
| 17 | Cl | 2.62 | 2.82 | X | X |

| Z # | | K α | K β | L α | L β |
|-----|----|------------|-----------|------------|-----------|
| 96 | Cm | 109.10 | 123.24 | 14.96 | 19.39 |
| 27 | Co | 6.93 | 7.65 | 0.78 | 0.79 |
| 24 | Cr | 5.41 | 5.43 | 0.57 | 0.58 |
| 55 | Cs | 30.97 | 34.98 | 4.29 | 4.62 |
| 29 | Cu | 8.05 | 8.90 | 0.93 | 0.95 |
| 66 | Dy | 45.99 | 52.18 | 6.50 | 7.25 |
| 68 | Er | 49.10 | 55.69 | 6.95 | 7.81 |
| 99 | Es | 117.65 | 132.78 | 16.02 | 21.17 |
| 63 | Eu | 41.53 | 47.03 | 5.85 | 6.46 |
| 9 | F | 0.677 | X | X | X |
| 26 | Fe | 6.40 | 7.06 | 0.70 | 0.72 |
| 100 | Fm | 120.60 | 136.08 | 16.38 | 21.79 |
| 87 | Fr | 86.12 | 97.48 | 12.03 | 14.77 |
| 64 | Gd | 42.98 | 48.97 | 6.06 | 6.71 |
| 31 | Ga | 9.25 | 10.26 | 1.10 | 1.12 |
| 32 | Ge | 9.89 | 10.98 | 1.19 | 1.21 |
| 1 | H | | | | |
| 105 | Ha | | | | |
| 2 | He | | | | |
| 72 | Hf | 55.76 | 63.21 | 7.90 | 9.02 |
| 80 | Hg | 70.82 | 80.26 | 9.99 | 11.82 |
| 67 | Ho | 47.53 | 53.93 | 6.72 | 7.53 |
| 53 | I | 28.61 | 32.29 | 3.94 | 4.22 |
| 49 | In | 24.21 | 27.27 | 3.29 | 3.49 |
| 77 | Ir | 64.89 | 73.55 | 9.19 | 10.71 |
| 19 | K | 3.31 | 3.59 | X | X |
| 36 | Kr | 12.65 | 14.11 | 1.59 | 1.64 |
| 57 | La | 33.44 | 37.80 | 4.65 | 5.04 |
| 3 | Li | 0.052 | X | X | X |

| Z # | | K α | K β | L α | L β |
|-----|----|------------|-----------|------------|-----------|
| 103 | Lr | | | | |
| 71 | Lu | 54.06 | 61.28 | 7.65 | 8.71 |
| 101 | Md | | | | |
| 12 | Mg | 1.25 | 1.30 | X | X |
| 25 | Mn | 5.90 | 6.49 | 0.64 | 0.65 |
| 42 | Mo | 17.48 | 19.61 | 2.29 | 2.40 |
| 7 | N | 0.392 | X | X | X |
| 11 | Na | 1.04 | 1.07 | X | X |
| 41 | Nb | 16.61 | 18.62 | 2.17 | 2.26 |
| 60 | Nd | 37.36 | 42.27 | 5.23 | 5.72 |
| 10 | Ne | 0.851 | X | X | X |
| 28 | Ni | 7.48 | 8.26 | 0.85 | 0.87 |
| 102 | No | | | | |
| 93 | Np | 101.00 | 114.18 | 13.95 | 17.74 |
| 8 | O | 0.526 | X | X | X |
| 76 | Os | 62.99 | 71.40 | 8.91 | 10.36 |
| 15 | P | 2.02 | 2.14 | X | X |
| 91 | Pa | 95.85 | 108.41 | 13.29 | 19.70 |
| 82 | Pb | 74.96 | 84.92 | 10.55 | 12.61 |
| 46 | Pd | 21.18 | 23.82 | 2.84 | 2.99 |
| 61 | Pm | 38.65 | 43.96 | 5.43 | 5.96 |
| 84 | Po | 79.30 | 89.81 | 11.13 | 13.44 |
| 59 | Pr | 36.02 | 40.75 | 5.03 | 5.49 |
| 78 | Pt | 66.82 | 75.74 | 9.44 | 11.07 |
| 94 | Pu | 103.65 | 117.15 | 14.28 | 18.28 |
| 88 | Ra | 88.46 | 100.14 | 12.34 | 15.23 |
| 37 | Rb | 13.39 | 14.96 | 1.69 | 1.75 |
| 75 | Re | 61.13 | 69.30 | 8.65 | 10.01 |
| 104 | Rf | | | | |

| Z # | | K α | K β | L α | L β |
|-----|----|------------|-----------|------------|-----------|
| 45 | Rh | 20.21 | 22.72 | 2.70 | 2.83 |
| 86 | Rn | 83.80 | 94.88 | 11.72 | 14.32 |
| 44 | Ru | 19.28 | 21.66 | 2.56 | 2.68 |
| 16 | S | 2.31 | 2.46 | X | X |
| 51 | Sb | 26.36 | 29.72 | 3.61 | 3.84 |
| 21 | Sc | 4.09 | 4.46 | 0.40 | X |
| 34 | Se | 11.22 | 12.50 | 1.38 | 1.42 |
| 106 | Sg | | | | |
| 14 | Si | 1.74 | 1.83 | X | X |
| 62 | Sm | 40.12 | 45.40 | 5.64 | 6.21 |
| 50 | Sn | 25.27 | 28.48 | 3.44 | 3.66 |
| 38 | Sr | 14.16 | 15.83 | 1.81 | 1.87 |
| 73 | Ta | 57.52 | 65.21 | 8.15 | 9.34 |
| 65 | Tb | 44.47 | 50.39 | 6.28 | 6.98 |
| 43 | Tc | 18.41 | 19.61 | 2.42 | 2.54 |
| 52 | Te | 27.47 | 30.99 | 3.77 | 4.03 |
| 90 | Th | 93.33 | 105.59 | 12.97 | 16.20 |
| 22 | Ti | 4.51 | 4.93 | 0.45 | 0.46 |
| 81 | Tl | 72.86 | 82.56 | 10.27 | 12.21 |
| 69 | Tm | 50.73 | 57.58 | 7.18 | 8.10 |
| 74 | W | 59.31 | 67.23 | 8.40 | 9.67 |
| 92 | U | 98.43 | 111.29 | 13.61 | 17.22 |
| 23 | V | 4.95 | 5.43 | 0.51 | 0.52 |
| 54 | Xe | 29.80 | 33.64 | 4.11 | 4.42 |
| 39 | Y | 14.96 | 16.74 | 1.92 | 2.00 |
| 70 | Yb | 52.36 | 59.35 | 7.41 | 8.40 |
| 30 | Zn | 8.64 | 9.57 | 1.01 | 1.03 |
| 40 | Zr | 15.77 | 17.67 | 2.04 | 2.12 |

COUNTING STATISTICS

Minimum Detectable Activity (MDA)

$$2k\sqrt{(R_B \times t_S + R_B \times t_B) / (t_S \times \text{Eff})}$$

Minimum Detectable Count Rate (MDCR = LLD = L_D)

$$2k\sqrt{(R_B \times t_S \times R_B \times t_B) / t_S}$$

$$L_C = k\sqrt{(R_B \times t_S + R_B \times t_B)}$$

k = sigma multiplier

t_S = sample count time

t_B = background count time

R_B = background count rate

Eff = efficiency of the detector (expressed as a decimal)

R_S = sample count rate

LLD is Lower Limit of Detection

L_D is the Decision Level

L_C is the Critical Level

MDA, MDCR, LLD, LD, and LC are generally expressed as signal level (or counts) above background

| | | | | |
|--------|------------|------------|------------|------------|
| K | 0.674 | 1.00 | 1.64485 | 1.95996 |
| % C.L. | 50.0 | 68.2689492 | 90.0 | 95.0 |
| K | 2.00 | 2.57583 | 2.80703 | 3.00 |
| % C.L. | 95.4499736 | 99.0 | 99.5 | 99.7300204 |
| K | 3.29053 | 4.00 | 5.00 | 6.00 |
| % C.L. | 99.9 | 99.9936658 | 99.9999427 | 99.9999998 |

If R_B is in DPM it must be converted to CPM and then multiplied by the count time to get accumulated counts.

A 'k' of 1.645 is used as the 95% confidence level for a two-tailed distribution.

Gaussian statistics should be used for ≥ 30 counts and Poisson statistics for < 30 counts.

Gaussian Formula

MDA when background and sample count times are one minute and k is 1.645. $2k\sqrt{(R_B \times t_S + R_B \times t_B) / (t_S \times \text{Eff})}$

$$2 \times 1.645 \sqrt{(C_B + C_B) / (t_S \times \text{Eff})} = 3.29 \sqrt{(2C_B) / (t_S \times \text{Eff})} = \\ 3.29 \times 1.414 \sqrt{(C_B) / (t_S \times \text{Eff})} = 4.65 \sqrt{(C_B) / (t_S \times \text{Eff})}$$

MDA when background count time is ten minutes and sample count time is one minute and k is 1.645.

$$2k\sqrt{(R_B \times t_S + R_B \times t_S / 10) / (t_S \times \text{Eff})}$$

$$2 \times 1.645 \sqrt{(R_B \times 1 + R_B \times 1/10) / (t_S \times \text{Eff})}$$

$$3.29 \sqrt{(1.1C_B) / (t_S \times \text{Eff})} = 3.29 \times 1.0488 \sqrt{(C_B) / (t_S \times \text{Eff})} = \\ 3.45 \sqrt{(C_B) / (t_S \times \text{Eff})}$$

To determine an action level or an alarm setpoint consider how many false positives are acceptable in a time frame.

Example: 100 Area Radiation Monitors (ARMs) are operating in a work area. The annual false alarm rate is 2 alarms in one year for all of the ARMs combined. The ARMs update and check for an alarm every minute. The combined ARMs check for the alarm condition 52,560,000 times each year. More than 2 false alarms in 52,560,000 checks is unacceptable. A 'K' of 6 (99.999998 % C.L.) is required.

POISSON STATISTICS

IF you have less than 30 counts then use Poisson statistics.

For Poisson distributions the following logic applies.

P_n is the probability of getting count "n"

$$P_n = \mu^n e^{-\mu} / n!$$

n = the hypothetical count

μ = true mean counts

If the true mean, μ , is 3, then there is a 5% probability that we will get a zero count and a 95% probability that we will get greater than zero counts. There is a 65% probability that we will get 3 or more counts.


α = Probability of Type I error (false positive)

β = Probability of Type II error (false negative)

$$B = B_{\text{kg}}$$

L_C = Critical level

L_D = Decision level

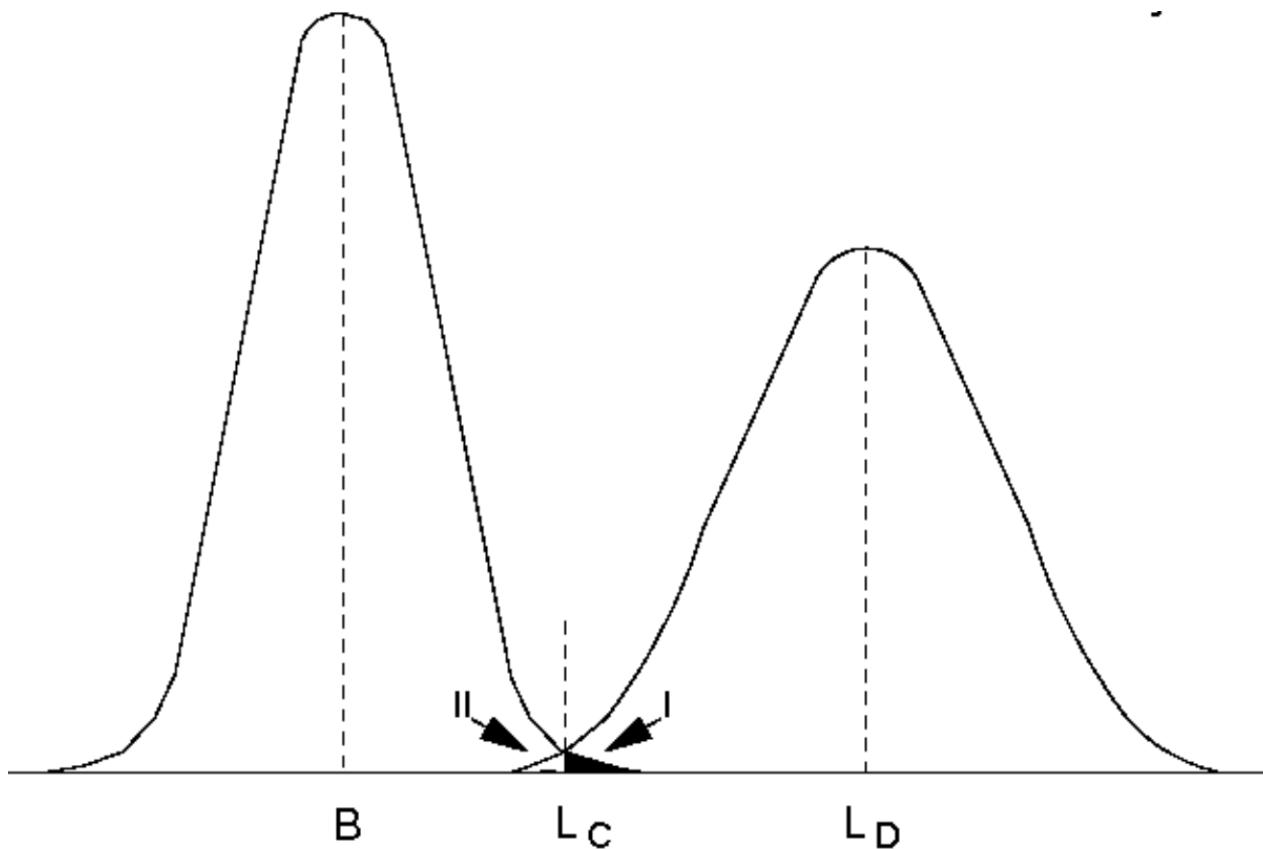

ELEVATION VS AIR PRESSURE

| Elevation | Barometric Pressure | | Boiling Point of Water | | Speed of Sound | | |
|-----------|---------------------|-----|------------------------|-------|----------------|-------|---------|
| | FT | M | mm Hg | kPa | °C | °F | M/S MPH |
| -500 | -152 | 774 | 103.2 | 100.5 | 212.9 | 340.9 | 763 |
| 0 | 0 | 760 | 101.3 | 100 | 212.0 | 340.3 | 761 |
| 500 | 152 | 746 | 99.5 | 99.5 | 211.1 | 339.7 | 760 |
| 1,000 | 305 | 732 | 97.6 | 99.0 | 210.2 | 339.1 | 759 |
| 1,500 | 457 | 720 | 96.0 | 98.4 | 209.2 | 338.6 | 757 |
| 2,000 | 610 | 707 | 94.3 | 97.9 | 208.3 | 338.0 | 756 |
| 2,500 | 762 | 694 | 92.5 | 97.4 | 207.4 | 337.4 | 755 |
| 3,000 | 914 | 681 | 90.8 | 97.0 | 206.6 | 336.7 | 753 |
| 3,500 | 1,067 | 668 | 89.1 | 96.4 | 205.6 | 336.2 | 752 |
| 4,000 | 1,219 | 656 | 87.5 | 95.9 | 204.6 | 335.6 | 751 |
| 4,500 | 1,372 | 644 | 85.9 | 95.4 | 203.7 | 334.8 | 749 |
| 5,000 | 1,524 | 632 | 84.3 | 94.9 | 202.9 | 334.4 | 748 |
| 5,500 | 1,676 | 619 | 82.5 | 94.4 | 202.0 | 333.8 | 747 |
| 6,000 | 1,829 | 609 | 81.2 | 93.9 | 201.1 | 333.2 | 745 |
| 6,500 | 1,981 | 597 | 79.6 | 93.3 | 200.0 | 332.6 | 744 |
| 7,000 | 2,134 | 586 | 78.1 | 92.8 | 199.1 | 332.2 | 743 |
| 7,500 | 2,286 | 575 | 76.7 | 92.4 | 198.3 | 331.4 | 741 |
| 8,000 | 2,438 | 564 | 75.2 | 91.8 | 197.4 | 330.8 | 740 |
| 9,000 | 2,743 | 543 | 72.4 | 90.9 | 195.6 | 330.1 | 738 |
| 10,000 | 3,048 | 523 | 69.7 | 89.8 | 193.7 | 328.5 | 735 |
| 11,000 | 3,353 | 504 | 67.1 | 88.8 | 191.4 | 327.3 | 732 |
| 12,000 | 3,658 | 484 | 64.5 | 87.8 | 190.1 | 326.0 | 729 |
| 13,000 | 3,962 | 464 | 62.0 | 86.8 | 188.2 | 324.6 | 726 |
| 14,000 | 4,267 | 444 | 59.5 | 85.8 | 186.4 | 323.2 | 723 |
| 15,000 | 4,572 | 424 | 57.0 | 84.8 | 184.6 | 321.8 | 720 |
| 16,000 | 4,877 | 404 | 54.6 | 83.7 | 182.7 | 320.4 | 717 |

ELEVATIONS OF MAJOR AIRPORTS AND FACILITIES

| | | Feet | | Feet |
|----|-------------|-------|----|----------------|
| AK | Anchorage | 144 | IL | Bloomington |
| AK | Fairbanks | 434 | IL | Moline |
| AL | Birmingham | 644 | IN | Bloomington |
| AL | Dothan | 401 | IN | Evansville |
| AL | Huntsville | 630 | KS | Wichita |
| AR | Little Rock | 260 | KY | Lexington |
| AR | Fort Smith | 469 | KY | Paducah |
| AZ | Flagstaff | 7,011 | LA | New Orleans |
| AZ | Phoenix | 1,133 | LA | Shreveport |
| AZ | Tucson | 2,641 | MA | Boston |
| CA | Imperial | -24 | MA | Worcester |
| CA | Lake Tahoe | 6,264 | MD | Hagerstown |
| CA | Sacramento | 24 | MD | Salisbury |
| CA | Los Angeles | 126 | ME | Portland |
| CO | Denver | 5,431 | ME | Presque Island |
| CO | Leadville | 9,927 | MI | Detroit |
| CO | Pueblo | 4,726 | MI | Hancock |
| CT | Bridgeport | 10 | MN | Duluth |
| CT | New Haven | 14 | MN | Minneapolis |
| DC | Washington | 313 | MO | Saint Louis |
| FL | Gainesville | 152 | MO | Springfield |
| FL | Miami | 11 | MS | Biloxi |
| GA | Atlanta | 1,026 | MS | Tupelo |
| GA | Savannah | 51 | MT | Yellowstone |
| HI | Honolulu | 13 | MT | Wolf Point |
| HI | Lanai City | 1,308 | NC | Asheville |
| IA | Burlington | 698 | NC | New Bern |
| IA | Mason City | 1,213 | ND | Grand Forks |
| ID | Idaho Falls | 4,741 | ND | Williston |
| ID | Lewiston | 1,438 | NE | Lincoln |

| | | | | | |
|----|---------------|-------|----|---------------------------|--------|
| NE | Omaha | 983 | UT | Cedar City | 5,623 |
| NH | Lebanon | 598 | UT | Saint George | 2,936 |
| NH | Manchester | 234 | UT | Salt Lake City | 4,227 |
| NJ | Atlantic City | 76 | VA | Norfolk | 27 |
| NJ | Trenton | 213 | VA | Roanoke | 1,176 |
| NM | Albuquerque | 5,352 | VT | Burlington | 334 |
| NM | Carlsbad | 3,293 | WA | Bellingham | 166 |
| NM | Los Alamos | 7,200 | WA | Pullman | 2,551 |
| NM | White Sands | 4,197 | WA | Richland | 195 |
| NV | Ely | 6,255 | WI | La Crosse | 654 |
| NV | Las Vegas | 2,175 | WI | Oshkosh | 808 |
| NY | Jamestown | 1,724 | WI | Rhineland | 1,623 |
| NY | New York | 13 | WV | Bluefield | 2,857 |
| OH | Akron | 1,228 | WV | Huntington | 828 |
| OH | Cincinnati | 897 | WY | Laramie | 7,276 |
| OH | Cleveland | 584 | WY | Sheridan | 4,021 |
| OK | Oklahoma City | 1,295 | | Lowest Spot in the US | |
| OK | Tulsa | 677 | | Death Valley, CA | -282 |
| OR | Portland | 27 | | | |
| OR | Redmond | 3,077 | | | |
| PA | Johnstown | 2,284 | | Highest Spot in the US | |
| PA | Philadelphia | 21 | | Mt. McKinley, AK | 20,320 |
| RI | Providence | 55 | | | |
| SC | Columbia | 236 | | | |
| SC | Myrtle Beach | 28 | | Lowest Spot in the World | |
| SD | Huron | 1,288 | | Dead Sea, Israel/Jordan | |
| SD | Rapid City | 3,202 | | | -1,371 |
| TN | Bristol | 1,519 | | | |
| TN | Memphis | 332 | | Highest Spot in the World | |
| TX | Dallas | 487 | | Mt. Everest, Nepal/China | |
| TX | El Paso | 3,956 | | | 29,035 |

INTERNATIONAL AIRPORT ELEVATIONS (FEET)

| | | | |
|----------------------------|--------|------------------------|-------|
| Addis-Ababa, Ethiopia | 7,625 | Montreal, Canada | 117 |
| Algiers, Algeria | 826 | Moscow, Russia | 623 |
| Amsterdam, Netherlands | -13 | Nairobi, Kenya | 5,327 |
| Athens, Greece | 90 | New Delhi, India | 776 |
| Bagdad, Iraq | 113 | Osaka, Japan | 39 |
| Beijing, China | 15 | Panama City, Panama | 135 |
| Berlin, Germany | 164 | Paris, France | 292 |
| Bogota, Columbia | 8,355 | Perth, Australia | 53 |
| Bombay, India | 27 | Port Moresby, | |
| Buenos Aires, Argentina | 66 | Papua New Guinea | 125 |
| Cairo, Egypt | 366 | Quito, Ecuador | 9,228 |
| Calgary, Canada | 3,557 | Recife, Brazil | 36 |
| Cape Town, South Africa | 151 | Reykjavik, Iceland | 169 |
| Casablanca, Morocco | 656 | Rio de Janeiro, Brazil | 16 |
| Damascus, Syria | 2,020 | Rome, Italy | 7 |
| Darwin, Australia | 94 | Santiago, Chili | 1,554 |
| Dublin, Ireland | 222 | Seoul, South Korea | 58 |
| Geneva, Switzerland | 1,411 | Shanghai, China | 15 |
| Helsinki, Finland | 167 | Shannon, Ireland | 47 |
| Istanbul, Turkey | 92 | Singapore, Singapore | 65 |
| Jakarta, Indonesia | 86 | Stockholm, Sweden | 123 |
| Johannesburg, South Africa | 5,557 | Sydney, Australia | 6 |
| Karachi, Pakistan | 100 | Taipei, Taiwan | 21 |
| Khartoum, Sudan | 1,256 | Tehran, Iran | 3,949 |
| La Paz, Bolivia | 13,354 | Tel Aviv, Israel | 135 |
| Lima, Peru | 105 | Tokyo, Japan | 8 |
| Lisbon, Portugal | 374 | Toronto, Canada | 569 |
| London, England | 80 | Tunis, Tunisia | 20 |
| Madrid, Spain | 1,998 | Vancouver, Canada | 8 |
| Manila, Phillipines | 74 | Warsaw, Poland | 361 |
| Melbourne, Australia | 392 | Zurich, Switzerland | 1,416 |
| Mexico City, Mexico | 7,341 | | |

COMPOSITION OF AIR

| | Symbol | % Volume | Density of Gases g / l |
|------------------|------------------|-----------------|-------------------------------|
| Air | - | 100.00 | 1.2928 |
| Nitrogen | N ₂ | 78.084 | 1.2506 |
| Oxygen | O ₂ | 20.947 | 1.4290 |
| Argon | Ar | 0.934 | 1.7840 |
| Carbon Dioxide | CO ₂ | 0.033 | 1.9770 |
| Neon | Ne | 18.2 PPM | 0.9002 |
| Helium | He | 5.2 PPM | 0.1785 |
| Methane | CH ₄ | 2.0 PPM | 0.66 |
| Krypton | Kr | 1.1 PPM | 3.7 |
| Sulfur Dioxide | SO ₂ | 1.0 PPM | 2.927 |
| Hydrogen | H ₂ | 0.5 PPM | 0.0899 |
| Nitrous Oxide | N ₂ O | 0.5 PPM | 1.977 |
| Xenon | Xe | 0.09 PPM | 5.9 |
| Ozone | O ₃ | 0.0 to 0.07 PPM | 2.144 |
| Ozone - winter | O ₃ | 0.0 to 0.02 PPM | 2.144 |
| Nitrogen Dioxide | NO ₂ | 0.02 PPM | 1.4494 |
| Iodine | I ₂ | 0.01 PPM | 4.93 |
| Carbon Monoxide | CO | 0.0 to trace | 1.2500 |
| Ammonia | NH ₃ | 0.0 to trace | 0.7710 |

SI and US “Traditional” Units

| Activity | | Dose Equivalent | |
|-----------------|---|------------------------|-----------------------------|
| 1 TBq | = | 27 Ci | 1 Sv = 100 rem |
| 1 GBq | = | 27 mCi | 1 mSv = 100 mrem |
| 1 MBq | = | 27 μ Ci | 1 mSv = 0.10 rem |
| 1 kBq | = | 27 nCi | 1 μ Sv = 100 μ rem |
| 1 Bq | = | 27 pCi | 1 μ Sv = 0.10 mrem |
| 1 Bq | = | 1 dps | 1 nSv = 0.10 μ rem |
| 1 Bq | = | 60 dpm | |
| 1 kCi | = | 37 TBq | 1 krem = 10 Sv |
| 1 Ci | = | 37 GBq | 1 rem = 10 mSv |
| 1 mCi | = | 37 MBq | 1 mrem = 10 μ Sv |
| 1 μ Ci | = | 37 kBq | 1 mrem = 0.01 mSv |
| 1 nCi | = | 37 Bq | 1 μ rem = 0.01 μ Sv |
| 1 nCi | = | 37 dps | 1 μ rem = 10 nSv |
| 1 nCi | = | 2220 dpm | |
| 1 pCi | = | 0.037 Bq | |
| 1 pCi | = | 2.22 dpm | |

Absorbed Dose

| | | |
|-------------|---|---------------|
| 1 kGy | = | 100 krad |
| 1 Gy | = | 100 rad |
| 1 mGy | = | 100 mrad |
| 1 μ Gy | = | 100 μ rad |
| | | |
| 1 krad | = | 10 Gy |
| 1 rad | = | 10 mGy |
| 1 mrad | = | 10 μ Gy |
| 1 μ rad | = | 10 nGy |

Dose Rate

| | | |
|---------------|---|-----------------|
| 1 Sv/h | = | 100 rem/h |
| 1 mSv/h | = | 100 mrem/h |
| 1 mSv/h | = | 0.10 rem/h |
| 1 μ Sv/h | = | 100 μ rem/h |
| 1 μ Sv/h | = | 0.1 mrem/h |
| 1 krem/h | = | 10 Sv/h |
| 1 rem/h | = | 10 mSv/h |
| 1 mrem/h | = | 10 μ Sv/h |
| 1 mrem/h | = | 0.01 mSv/h |
| 1 μ rem/h | = | 0.01 μ Sv/h |

ABBREVIATIONS

| | |
|----------------------------|------------------------------|
| ampere | A, or amp |
| angstrom unit | A, or Å |
| atmosphere | atm |
| atomic weight | at. wt. |
| becquerel | Bq |
| cubic foot | ft ³ , or cu ft |
| cubic feet per minute | ft ³ /min, or cfm |
| cubic inch | in ³ , or cu. in. |
| cubic meter | m ³ , or cu m |
| curie | Ci |
| day | day, or d |
| degree | deg, or ° |
| disintegrations per minute | dpm |
| foot | ft |
| gallon | gal |
| gallons per minute | gpm |
| gram | g or gm |
| hour | h, or hr |
| inch | in. |
| liter | liter, or L |
| meter | m |
| micron | μ, μm, or mu |
| minute | min, or m |
| pounds per square inch | lb/in ² , or psi |
| roentgen | R |
| second | sec, or s |
| square centimeter | cm ² , or sq cm |
| square foot | ft ² , sq ft |
| square meter | m ² , or sq m |
| volt | V, or v |
| watt | W, or w |
| year | yr, or y |

CONVERSION OF UNITS

Length

| | | | | | |
|-------------------------------------|---|---------------|--------|---|-------------------|
| 1 angstrom (\AA) | = | 1E-8 cm | 1 cm | = | 1E8 \AA |
| 1 inch | = | 2.54 cm | 1 cm | = | 0.3937 in |
| 1 meter | = | 3.2808 feet | 1 foot | = | 0.3048 m |
| 1 kilometer | = | 0.6214 miles | 1 mile | = | 1.609 km |
| 1 mile | = | 5,280 feet | 1 foot | = | 1.894E-4 mi |
| 1 micron (μm) | = | 1E-6 meters | 1 m | = | 1E6 μm |
| 1 mil | = | 1E-3 inches | 1 inch | = | 1E3 mil |
| 1 thousandth of an inch (0.001") | = | 2.54E-2 mm | 1 mm | = | 0.03937 in |
| 1 yard | = | 0.9144 meters | 1 m | = | 1.0936 yard |

Area

| | | | | | |
|-------------------|---|--------------------------|-------------------|---|-------------------------|
| 1 acre | = | 43,560 ft^2 | 1 ft^2 | = | 2.296E-5 acre |
| 1 barn | = | 1E-24 cm^2 | 1 cm^2 | = | 1E24 barn |
| 1 cm^2 | = | 0.1550 in^2 | 1 in^2 | = | 6.452 cm^2 |
| 1 m^2 | = | 10.764 ft^2 | 1 ft^2 | = | 0.0929 m^2 |
| 1 m^2 | = | 3.861E-7 mile^2 | 1 mile^2 | = | 2.59E6 m^2 |
| 1 mile^2 | = | 640 acres | 1 acre | = | 1.5625E-3 mi^2 |

Volume

| | | | | | |
|----------------------|---|-------------------------|-----------------|---|------------------------|
| 1 cm^3 (cc) | = | 3.5315E-5 ft^3 | 1 ft^3 | = | 28,316 cm^3 |
| 1 cm^3 | = | 1E-6 m^3 | 1 m^3 | = | 1E6 cm^3 |
| 1 cm^3 | = | 0.03381 ounces | 1 ounce | = | 29.58 cm^3 |
| 1 ft^3 | = | 28.316 liters | 1 liter | = | 0.035315 ft^3 |
| 1 ft^3 | = | 7.481 gallons | 1 gal | = | 0.1337 ft^3 |
| 1 liter | = | 1.057 quarts | 1 quart | = | 0.946 liter |
| 1 liter | = | 0.2642 gallons | 1 gal | = | 3.785 liter |
| 1 liter | = | 61.0237 in^3 | 1 in^3 | = | 0.016387 liter |
| 1 m^3 | = | 35.315 ft^3 | 1 ft^3 | = | 0.028316 m^3 |
| 1 m^3 | = | 1,000 liters | 1 liter | = | 1E-3 m^3 |
| 1 milliliter (ml) | = | 1 cm^3 | 1 cm^3 | = | 1 ml |

Mass

| | | | | | |
|------------|---|----------------|---------|---|--------------|
| 1 gram | = | 0.03527 ounces | 1 ounce | = | 28.35 g |
| 1 kilogram | = | 2.2046 pounds | 1 lbs | = | 0.4536 kg |
| 1 pound | = | 16 ounces | 1 ounce | = | 0.0625 lb |
| 1 pound | = | 453.59 grams | 1 gram | = | 2.2046E-3 lb |

Density

| | | | | | |
|--------------------------|---|------------------------------|----------------------|---|----------------------------|
| 1 gram / cm ³ | = | 62.428 lbs / ft ³ | 1 lb/ft ³ | = | 0.016018 g/cm ³ |
| 1 gram / cm ³ | = | 8.345 lbs / gal | 1 lb/gal | = | 0.1198 g/cm ³ |

Concentration

| | | | | | |
|-------------------------|---|---------------------------------|----------------------|---|--------------------------|
| 1 Bq / M ³ | = | 60 DPM / M ³ | 1 DPM/M ³ | = | 0.0167 Bq/M ³ |
| 1 Bq / M ³ | = | 0.027027pCi/L | 1 pCi / L | = | 37 Bq / M ³ |
| 1 pCi / L | = | 1E-9 µCi / cc | 1 µCi / cc | = | 1E9 pCi / L |
| 1 µCi / cc | = | 2.22E12 DPM/M ³ | | | |
| 1 DPM / M ³ | = | 4.5045E-13 µCi/cc | | | |
| 1 µCi / cc | = | 3.7E10 Bq / M ³ | | | |
| 1 Bq / M ³ | = | 2.7027E-11 µCi/cc | | | |
| 1 pCi / ft ³ | = | 3.5315E-11 µCi / cc | | | |
| 1 µCi / cc | = | 2.8316E10 pCi / ft ³ | | | |

Pressure

| | | | | | |
|------------------------|---|-------------------------------|-------------------------|---|-----------------------------|
| 1 atmosphere | = | 1.01325 bars | 1 bar | = | 0.9869 atm |
| 1 atmosphere | = | 101.325 kPa | 1 kPa | = | 0.009869 atm |
| 1 atmosphere | = | 14.696 lbs / in ² | 1 lbs / in ² | = | 0.06805 atm |
| 1 atmosphere | = | 760 mm Hg | 1 mm Hg | = | 0.001316 atm |
| 1 atmosphere | = | 29.9213 "Hg | 1 "Hg | = | 0.033421 atm |
| 1 atmosphere | = | 33.8995 feet H ₂ O | 1 ft H ₂ O | = | 0.0295 atm |
| 1 bar | = | 1E6 dynes / cm ² | 1 dyne/cm ² | = | 1E-6 bar |
| 1 dyne/cm ² | = | 0.1 Pascals | 1 Pascal | = | 10 dyne/cm ² |
| 1 Torr | = | 1 mm Hg | 1 mm Hg | = | 1 Torr |
| 1 dyne/cm ² | = | 1.0197E-3 g/cm ² | 1 g/cm ² | = | 980.68 dyne/cm ² |

Radiological

| | | |
|--------------------------------|---|--------------------------------------|
| 1 rad | = | 100 ergs / g |
| 1 erg / g | = | 0.01 rad |
| 1 rad | = | 6.242E13 eV / g |
| 1 eV / g | = | 1.602E-13 roentgen |
| 1 roentgen | = | 87.7 ergs / g of air |
| 1 erg / g of air | = | 0.0114 roentgen |
| 1 roentgen | = | 1.61E12 ion pairs/g of air |
| 1 ion pair / g of air | = | 6.21E-13 roentgen |
| 1 roentgen | = | 5.47E13 eV / g of air |
| 1 eV / g of air | = | 1.828E-14 roentgen |
| 1 roentgen | = | 0.98 rads (in soft tissue) |
| 1 rad (in soft tissue) | = | 1.02 roentgen |
| 1 rem | = | 100 ergs / g in tissue |
| 1 erg /g in tissue | = | 0.01 rem |
| 1 sievert (Sv) | = | 100 rem |
| 1 rem | = | 0.01 Sv |
| 1 sievert | = | 1 J / kg |
| 1 curie (Ci) | = | 3.7E10 dps |
| 1 dps | = | 2.7027E-11 Ci |
| 1 curie | = | 2.22E12 dpm |
| 1 dpm | = | 4.5045E-13 Ci |
| 1 $\mu\text{Ci} / \text{m}^2$ | = | 222 dpm / cm ² |
| 1 dpm / cm ² | = | 0.0045 $\mu\text{Ci} / \text{m}^2$ |
| 1 megaCi / sq mile | = | 0.386 Ci / m ² |
| 1 Ci / m ² | = | 2.59 megaCi/sq mile |
| 1 dpm / m ³ | = | 4.5E-13 $\mu\text{Ci} / \text{cm}^3$ |
| 1 $\mu\text{Ci} / \text{cm}^3$ | = | 2.22E12 dpm / m ³ |
| 1 becquerel (Bq) | = | 2.7027E-11 Ci |
| 1 Ci | = | 3.7E10 Bq |
| 1 becquerel | = | 1 dps |
| 1 dps | = | 1 Bq |

Radiological

| | | |
|--------------------------------|---|--------------------------------------|
| 1 BTU | = | 1.28E-8 g U ²³⁵ fissioned |
| 1 g U ²³⁵ fissioned | = | 7.81E7 BTU |
| 1 BTU | = | 3.29E13 fissions |
| 1 fission | = | 3.04E-14 BTU |
| 1 g U ²³⁵ fissioned | = | 1 megawatt-days |
| 1 MW-days | = | 1 g U ²³⁵ fissioned |
| 1 g U ²³⁵ fissioned | = | 1.8E-2 kilotons TNT |
| 1 kilotons TNT | = | 55.6 g U ²³⁵ fissioned |
| 1 fission | = | 8.9058E-18 kW-hours |
| 1 kW-hrs | = | 1.123E17 fissions |
| 1 fission | = | 3.204E-4 ergs |
| 1 erg | = | 3.121E3 fissions |
| 1 fission | = | 6.9E-21 Megatons TNT |
| 1 Megatons TNT | = | 1.45E20 fissions |
| 1 gray | = | 100 rads |
| 1 rad | = | 0.01 gray |
| 1 joule (J) | = | 6.24E18 eV |
| 1 eV | = | 1.602E-19 joule |

Others

| | | |
|---------------------|---|---------------------------------|
| 1 ampere | = | 2.998E9 electrostatic units/sec |
| 3.336E-10 amp | = | 1 electrostatic unit/sec |
| 1 ampere | = | 6.242E18 electronic charges/sec |
| 1.602E-19 amp | = | 1 electronic charge/sec |
| 1 coulomb | = | 6.242E18 electronic charges |
| 1 electronic charge | = | 1.602E-19 coulomb |

Power

| | | | | | | |
|--------------|---|--------------|--|-------------|---|-------------------|
| 1 joule/sec | = | 1E7 ergs/sec | | 1 erg/sec | = | 1E-7 joule/sec |
| 1 watt | = | 1E7 ergs/sec | | 1 erg/sec | = | 1E-7 watt |
| 1 watt | = | 1 joule/sec | | 1 joule/sec | = | 1 watt |
| 1 watt | = | 0.001341 hp | | 1 hp | = | 745.7 watts |
| 1 BTU/min | = | 0.01757 kW | | 1 kW | = | 56.9 BTU/min |
| 1 BTU/min | = | 0.023575 hp | | 1 hp | = | 42.4 BTU/min |
| 1 joule | = | 9.478E-4 BTU | | 1 BTU | = | 1.055E3 joules |
| 1 joule | = | 1E7 ergs | | 1 erg | = | 1E-7 joule |
| 1 calorie, g | = | 0.003971 BTU | | 1 BTU | = | 251.8 calories, g |

MULTIPLES AND SUBMULTIPLES

| | | | | | | | | |
|------|------|---|------|-------|----|-------|-------|-------|
| 1E18 | Exa | E | 1E2 | hecto | h | 1E-6 | micro | μ |
| 1E15 | Peta | P | 1E1 | deka | da | 1E-9 | nano | n |
| 1E12 | tera | T | 1E0 | 1 | 1 | 1E-12 | pico | p |
| 1E9 | giga | G | 1E-1 | deci | d | 1E-15 | femto | f |
| 1E6 | mega | M | 1E-2 | centi | c | 1E-18 | atto | a |
| 1E3 | kilo | k | 1E-3 | milli | m | | | |

GREEK ALPHABET

| | | | | | | | | |
|----------|------------|---------|-----------|-----------|---------|------------|------------|---------|
| A | α | Alpha | I | ι | Iota | P | ρ | Rho |
| B | β | Beta | K | κ | Kappa | Σ | σ | Sigma |
| Γ | γ | Gamma | Λ | λ | Lambda | \Tau | τ | Tau |
| Δ | δ | Delta | M | μ | Mu | Υ | υ | Upsilon |
| E | ϵ | Epsilon | N | ν | Nu | Φ | ϕ | Phi |
| Z | ζ | Zeta | Ξ | ξ | Xi | \Chi | χ | Chi |
| H | η | Eta | O | \circ | Omicron | Ψ | ψ | Psi |
| Θ | θ | Theta | Π | π | Pi | Ω | ω | Omega |

CONSTANTS

| | |
|---|---|
| Avogadro's number (N_0) | 6.02252E23 |
| electron charge (e) | 4.80298E-10 esu |
| e electron rest mass (m) | 9.1091E-28 g |
| acceleration of gravity (g) | 32.1725 ft / sec ² |
| @ sea level & 45 ⁰ latitude | 980.621 cm / sec ² |
| Planck's constant (h) | 6.625E-27 erg-sec |
| velocity of light (c) | 2.9979E10 cm / sec 186,280 miles / sec |
| ideal gas volume (V_0) | 22,414 cm ³ / mole (STP) |
| neutron mass | 1.67482E-24 g |
| proton mass | 1.67252E-24 g |
| ratio of proton to electron mass | 1836.13 |
| natural base of logarithms (e) | 2.71828 |
| pi | 3.14159 |
| 1C | 6.2418E18 esus |
| 1A | 1 C/sec |
| 1 barn (b) | 1E-24 cm ² |
| charge (e-1) | 1.6E-19 C |
| W for air | 33.8 eV / ion pair |
| Universal gas constant (R) | 8.32E7 ergs/ ⁰ C gram mol |
| A gram-molecular weight of any gas contains Avogadro's number, N_0 (6.02252E23) atoms and occupies a volume of 22,414 cm ³ at STP. | |

Temperature

$$\begin{aligned}
 {}^0\text{C} &= ({}^0\text{F} - 32)(5/9) & {}^0\text{F} &= {}^0\text{C} \times 1.8 + 32 \\
 \text{K (Kelvin)} &= {}^0\text{C} + 273.15 & {}^0\text{R (Rankine)} &= {}^0\text{F} + 459.58 \\
 \text{Absolute zero is } 0 \text{ Kelvin, } 0 {}^0\text{R, } -273.15 {}^0\text{C, } -459.67 {}^0\text{F}
 \end{aligned}$$

SURFACE AREA AND VOLUME CALCULATIONS

Triangle $A \text{ (area)} = \frac{1}{2} \times b \times h$;
where b is the base and h is the height of the triangle

Rectangle $A \text{ (area)} = a \times b$;
where a and b are the lengths of the sides

Rectangular Box $V \text{ (volume)} = w \times l \times h$;
where w is the width, l is the length, and h is the height

Parallelogram (a 4-sided figure with opposite sides parallel)
 $A \text{ (area)} = a \times h$; or $a \times b \times \sin \Theta$;
where a and b are the length of the sides, h is the altitude (or vertical height), and Θ is the angle between the sides

Trapezoid (a 4-sided figure with two sides parallel)
 $A \text{ (area)} = \frac{1}{2} \times h (a + b)$;
where a and b are the length of the sides and h is the height

Regular polygon of n sides
 $A \text{ (area)} = \frac{1}{4} \times n \times a^2 \times \cot(180^\circ / n)$;
where a is the length of a side and n is the number of sides

Circle $A \text{ (area)} = \pi r^2$; or $\frac{1}{4} \pi d^2$;
where r is the radius and d is the diameter

Cube $A \text{ (area)} = 6 \times a^2$; $V \text{ (volume)} = a^3$;
where a is the length of a side

Cylinder $A \text{ (area)} = 2 \pi r h$; $V \text{ (volume)} = \pi r^2 h$;
where r is the radius and h is the length of the height

Sphere $A \text{ (area)} = 4 \pi r^2$; or πd^2 ; $V \text{ (volume)} = \frac{4}{3} \pi r^3$ or $\frac{1}{6} \pi d^3$
where r is the radius and d is the diameter

ELECTROMAGNETIC SPECTRUM

| Wavelength Meters | Frequency MHz | Energy keV | Radiation Type |
|--|------------------|------------------|--------------------------|
| 1E-8 | 3E20 | 1.24E9 | Cosmic |
| 1E-14 | 3E16 | 1.24E5 | X-Ray |
| 1E-10 | 3E12 | 1.24E1 | gamma |
| 1E-6 | 3E8 | 1.24E-3 | UV |
| 1E-2 | 3E4 | 1.24E-7 | IR |
| 1E2 | 3 | 1.24E-11 | visible |
| 1E6 | 3E-4 | 1.24E-15 | microwave radar TV |
| λ (meters wavelength) = $300 / F$ | | = 1.24E-9 / keV | |
| F (frequency MHz) = $300 / \lambda$ | | = 2.419E11 x keV | |
| E (keV) = $1.24E-9 / \lambda$ = $F / 2.419E11$ | | | |

The diagram illustrates the Electromagnetic Spectrum with horizontal lines representing different regions. Arrows point from the table entries to these regions. The regions are labeled: Cosmic, X-Ray, gamma, UV, visible, IR, microwave radar TV, and TV shortwave radio.

RULES OF THUMB FOR ALPHA PARTICLES

1. An alpha particle of at least 7.5 MeV energy is needed to penetrate the nominal protective layer of the skin (7 mg / cm^2 or 0.07 mm).
2. The alpha emissions and energies of the predominant particles from 1 μg of several common materials are:

| | DPM per μg | Alpha Energy (MeV) |
|----------------------------------|---|---------------------------|
| Pu-238 | 39,000,000 | 5.50 (72%) |
| Pu-239 | 140,000 | 5.15 (72.5%) |
| Pu-240 | 500,000 | 5.16 (76%) |
| Pu-242 | 8,700 | 4.90 (76%) |
| ^a Natural U | 1.5 | 4.20 (37%), 4.77 (36%) |
| Oralloy (93% 235U) | 160 | 4.39 (~ 80%) |
| ^b Natural Th | 0.5 | 4.01 (38%), 5.43 (36%) |
| ^c D-38 (DU, tuballoy) | 1 | 4.20 (~ 60%) |

^a Includes 234U in equilibrium

^b Includes 228Th in equilibrium. Depending upon the time since chemical separation, 228Th can decrease to give a net disintegration rate lower than 0.5.

^c With 2pi (50%) geometry, the surface of a thick uranium metal (tuballoy) source gives ~ 2400 alpha counts/min per cm^2 .

Depleted uranium (D-38) gives ~ 800 alpha cpm/ cm^2 .

3. Alpha particles lose about 0.8 MeV per mg/cm^2 density thickness of the attenuating material.
4. Detector window thicknesses cause alpha particles to lose energy at about 0.8 MeV per mg/cm^2 of window thickness. Therefore, a detector with a window thickness of 3 mg/cm^2 (such as sealed gas-proportional pancake alpha/beta detectors and pancake GM detectors) will not detect alpha emitters of less than 3 MeV.

5. Air-proportional alpha detectors have a flatter energy vs efficiency response than sealed gas-proportional, alpha scintillator, alpha/beta scintillator, or GM detectors. This is due to several factors. One factor is the typically thinner entrance windows on air-proportional alpha detectors compared to beta detectors and alpha and beta scintillator detectors whereby more of the initial alpha particle energy enters the active volume of the air-proportional compared to other detectors. A second factor is the relatively shallow depth of the air-proportional detector compared to the path length of the alpha particle in air which leads to the alpha pulses being of similar height for any alpha particle energy above a threshold.

6. **Alpha particle energy transfer to air**

6 MeV alpha particles produce 40,000 Ion Pairs per cm

4 MeV alpha particles produce 55,000 Ion Pairs per cm

ω for air is 34 eV per Ion Pair

therefore;

6 MeV alpha particles lose 1.18 MeV per cm of air

4 MeV alpha particles lose 1.87 MeV per cm of air

Alpha particle range in cm of air at 1 atmosphere

$$R = 0.56 E \text{ (} E < 4 \text{ MeV)}$$

$$R = 1.24 E - 2.62 \text{ (} E > 4 \text{ MeV)}$$

Alpha particles lose about 60 KeV of energy per mm of air at STP.

RULES OF THUMB FOR BETA PARTICLES

1. Beta particles of at least 70 keV energy are required to penetrate the nominal protective layer of the skin.
2. The average energy of a beta-ray spectrum is approximately one-third the maximum energy.
3. The range of beta particles in air is ~ 12 ft (3.6 m) / MeV.
4. The range of beta particles (or electrons) in grams / cm^2 (thickness in cm multiplied by the density in g / cm^3) is approximately half the maximum energy in MeV. This rule overestimates the range for low energies (0.5 MeV) and low atomic numbers, and underestimates for high energies and high atomic numbers.
5. The exposure rate in rads per hour in an infinite medium uniformly contaminated by a beta emitter is $2.12 EC / \rho$ where E is the average beta energy per disintegration in MeV, C is the concentration in $\mu\text{Ci} / \text{cm}^3$, and ρ is the density of the medium in grams / cm^3 . The dose rate at the surface of the mass is one half the value given by this relationship. In such a large mass, the relative beta and gamma dose rates are in the ratio of the average energies released per disintegration.
6. The surface dose rate through 7 mg / cm^2 from a uniform thin deposition of 1 mCi / cm^2 is about 9 rad/h (90 mGy/h) for energies above about 0.6 MeV. Note that in a thin layer, the beta dose rate exceeds the gamma dose rate for equal energies released by ~ 100 .

- 7.** The bremsstrahlung from a 1 Ci P-32 aqueous solution in a glass bottle is ~ 3 mrad/h (30 μ Gy/h) at 1 m.

8. Half-value thickness vs beta energy

| Isotope | β^- max energy (KeV) | Half-Value Thickness |
|---------|--|--------------------------|
| Tc-99 | 292 | 7.5 mg / cm ² |
| Cl-36 | 714 | 15 mg / cm ² |
| Sr/Y-90 | 546 / 2270 | 150 mg / cm ² |
| U-238 | Betas from short lived progeny 191 / 2290 | 130 mg / cm ² |

9. Estimating beta energy using a paper shield

- a) The density thickness of typical notepaper of 20 pound weight is 7.5 mg/cm².
- b) Take a reading with your beta detector of the surface contamination you wish to estimate the energy of.
- c) A single sheet of notepaper will stop all but the most energetic of alpha particles, will have virtually no effect on gamma radiation, and will only stop very low energy beta particles such as C-14.
- d) A single sheet of notepaper will reduce the count rate from Tc-99 by $\frac{1}{2}$.
- e) Continue adding more sheet of notepaper until the net count rate is less than $\frac{1}{2}$ the unshielded count rate.
- f) Multiply the number of sheet of notepaper necessary to reduce the count rate to $\frac{1}{2}$ by 7.5 mg/cm². That density thickness is your half-value layer and you can compare the required density thickness with the table in step 8 or some other reference.

RULES OF THUMB FOR GAMMA RADIATION

1. The range of gamma rays (any photon) for energies from eV to 10 MeV in air is from a few mm to 100 meters. The range of those photons in water is from a few mm to several cm.
2. The dose rate 1 m above a flat, infinite plane contaminated with a thin layer ($1 \text{ Ci} / \text{m}^2$) of gamma emitters is:

| Energy (MeV) | Dose Rate | |
|--------------|-----------|-------|
| | rem/h | mSv/h |
| 0.4 | 7.2 | 72 |
| 0.6 | 10 | 100 |
| 0.8 | 13 | 130 |
| 1.0 | 16 | 160 |
| 1.2 | 19 | 190 |

3. The dose rate in rem/h per hour in an infinite medium uniformly contaminated by a gamma emitter is $2.12 EC / \rho$, where C is the number of microcuries per cubic centimeter, E is the average gamma energy per disintegration in MeV, and ρ is the density of the medium. At the surface of a large body, the dose rate is about half of this. At ground level (one-half of an infinite cloud), the dose rate from a uniformly contaminated atmosphere is $1,600 EC \text{ rem/h per mCi / cm}^3$.
4. The radiation scattered from the air (skyshine) from a 100 Ci Co-60 source 30 cm behind a 1 m high shield is $\sim 100 \text{ mR/h}$ (1 mSv/h) at 15 cm from the outside of the shield.

RULES OF THUMB FOR NEUTRONS

1. The number of neutrons per square centimeter per second at distance R from a small source emitting Q neutrons per second without shielding is given by;
$$n / \text{cm}^2\text{-sec} = Q / 4\pi R^2 = 0.08Q / R^2$$
2. For α , η sources use the following equation to approximate the number of neutrons per second per Ci (Q).
$$Q = 5.6E3 \times (\text{alpha particle energy in MeV})^{3.65}$$
This holds true for Be; multiply by 0.16 for B targets, by 0.05 for F, by 0.015 for Li, and 0.003 for O targets.
3. For neutron energies from 1 to 10 MeV the neutron exposure rate is approximately equal to 1 mrem/hr at 1 meter for each $1E6$ neutrons per second emission rate. Multiply the neutron mrem/hr at 1 meter by 11.1 to calculate the neutron exposure rate for the same source at a distance of 30 cm.
4. For spontaneous fission the gamma exposure rate for an unshielded source is approximately twice the neutron exposure rate.
5. The range of neutrons in air for energies from 0 to 10 MeV is from a few centimeters to 100 meters.
6. The range of neutrons in water (or tissue) for energies from 0 to 10 MeV is from a few millimeters to 1 meter.
7. Neutron flux to dose rate conversion:
Fast: $1 \text{ mrem (0.01 mSv) / hr per } 6 \text{ n / cm}^2\text{-sec}$
Slow: $1 \text{ mrem (0.01 mSv) / hr per } 272 \text{ n / cm}^2\text{-sec}$

APPROXIMATE NEUTRON ENERGIES

| | |
|---------------|----------------|
| cold neutrons | 0 - 0.025 eV |
| thermal | 0.025 eV |
| epithermal | 0.025 - 0.4 eV |
| cadmium | 0.4 - 0.6 eV |
| epicadmium | 0.6 - 1 eV |
| slow | 1 eV - 10 eV |
| resonance | 10 eV - 300 eV |
| intermediate | 300 eV - 1 MeV |
| fast | 1 MeV - 20 MeV |
| relativistic | > 20 MeV |

Note: A thermal neutron is one which has the same energy and moves at the same velocity as a gas molecule does at a temperature of 20 degrees C. The velocity of a thermal neutron is 2200 m / sec (~5,000 mph).

Neutron Fluence per mrem (10CFR20)

| MeV | n/cm ² | | n/cm ² /s | | n/cm ² | |
|---------|-------------------|-------|----------------------|---------|-------------------|-------|
| | per | mrem | per | mrem/hr | per | mrem |
| thermal | | | | | 10 | 2.4E4 |
| to | 9E5 | 250 | | | 14 | 1.7E4 |
| 1E-2 | | | | | 20 | 1.6E4 |
| 1E-1 | 1.7E5 | 47 | | | 40 | 1.4E4 |
| 5E-1 | 3.9E4 | 11 | | | 60 | 1.6E4 |
| 1 | 2.7E4 | 7.5 | | | 100 | 2E4 |
| 2.5 | 2.9E4 | 8 | | | 200 | 1.9E4 |
| 5 | 2.3E4 | 6.4 | | | 300 | 1.6E4 |
| 7 | 2.4E4 | 6.7 | | | 400 | 1.4E4 |

Spontaneous Fission Neutron and Gamma Yields

| | SF (years) | n/s/Ci | n/s/GBq | neutron | gamma mrem / hr per Ci @ 30 cm |
|--------|------------|--------|---------|---------|--------------------------------------|
| | half-life | | | | |
| Es-253 | 6.7E5 | 7.14E3 | 1.92E2 | 0.1 | 0.1 |
| Cf-252 | 85 | 2.64E9 | 7.14E7 | 2.93E4 | 1E4 |
| Bk-249 | 6E8 | 1.25E2 | 3.38 | <0.1 | <0.1 |
| Cm-244 | 1.38E7 | 1.11E5 | 3.0E3 | 1.2 | 0.4 |
| Cm-242 | 7.2E6 | 5.28E3 | 1.43E2 | <0.1 | 0.1 |
| Am-241 | 2E14 | 0.18 | 4.86E-3 | <0.1 | <0.1 |
| Pu-242 | 7E10 | 4.56E5 | 1.23E4 | 5.0 | 2.0 |
| Pu-240 | 1.39E11 | 4.01E3 | 1.08E2 | <0.1 | 0.1 |
| Pu-239 | 5.5E15 | 0.37 | 1.0E-2 | <0.1 | <0.1 |
| Pu-238 | 4.9E10 | 1.52E2 | 4.1 | <0.1 | <0.1 |
| Pu-236 | 3.5E9 | 69.7 | 1.88 | <0.1 | <0.1 |
| Np-237 | 1E18 | 0.18 | 4.86E-3 | <0.1 | <0.1 |
| U-238 | 7E15 | 5.44E4 | 1.47E3 | 0.6 | 0.2 |
| U-235 | 1.9E17 | 3.15E2 | 8.51 | <0.1 | <0.1 |
| U-234 | 2E16 | 1.05 | 2.84E-2 | <0.1 | <0.1 |
| U-232 | 8E13 | 0.07 | 1.89E-3 | <0.1 | <0.1 |
| Th-232 | 1E21 | 1.18 | 3.19E-2 | <0.1 | <0.1 |

These neutron and gamma exposure rates are approximate values for the spontaneous fission process. When you are making exposure rate measurements you should take into account shielding of the source (including self-shielding), individual instrument response to both neutron and gamma radiation, isotopic mixtures, age of the material (for both decay and ingrowth), homogeneity of the material, and impurities. Refer to the Specific Activity and Characteristic Radiations of Commonly Encountered Radionuclides sections for information on gamma exposure rates and radiations from primary decay modes of these isotopes.

Energy & Yield of neutrons from the alpha, n reaction

neutron

| | η energy MeV | n/s/GBq | n/s/Ci | mrem/hr per Ci @ 30 cm |
|--|----------------------|---|---------|---------------------------|
| Cf ²⁵² O | 4.5 | 8.73E6 | 3.23E8 | 3,600 |
| Cm ²⁴⁴ Be | 4 | 1.0E5 | 3.7E6 | 41.1 |
| Cm ²⁴⁴ O | 1.9 | 1.0E5 | 3.7E6 | 41.1 |
| Cm ²⁴² Be | 4 | 1.12E5 | 4.1E6 | 45.5 |
| Cm ²⁴² O | 1.9 | 1.12E5 | 4.1E6 | 45.5 |
| Am ²⁴¹ Be | 4.5 | 7.6E4 | 2.8E6 | 34.7 |
| Am ²⁴¹ B | 2.8 | 1.3E4 | 4.8E5 | 5.9 |
| Am ²⁴¹ F | 1.3 | 4.1E3 | 1.5E4 | 0.17 |
| Am ²⁴¹ Li | 0.7 | 1.4E3 | 5.2E4 | 0.29 |
| Am ²⁴¹ O | 1.9 | 250 | 9.23E3 | 0.1 |
| Pu ²⁴² O | 1.7 | 2.13E-4 | 7.88E-3 | 8.7E-8 |
| Pu ²⁴⁰ O | 1.9 | 0.86 | 32 | 3.6E-4 |
| Pu ²³⁹ Be | 4.5 | 6.1E4 | 2.3E6 | 28.5 |
| Pu ²³⁹ O | 1.9 | 0.06 | 2.36 | 2.6E-5 |
| Pu ²³⁸ Be | 4.5 | 7.9E4 | 2.9E6 | 32.2 |
| Pu ²³⁸ O | 1.9 | 6.19E3 | 2.29E5 | 2.5 |
| Pu ²³⁹ F | 1.4 | 5.4E3 | 2E5 | 2.2 |
| Pu ²³⁸ Li | 0.6 | 38 | 1.4E3 | 0.008 |
| Pu ²³⁸ C ¹³ | 3.6 | 1.1E4 | 4.1E4 | 0.46 |
| Pu ²³⁶ O | 2.0 | 54 | 2E3 | 0.02 |
| Np ²³⁷ O | 1.2 | 54 | 2E3 | 0.02 |
| U ²³⁸ O, U ²³⁵ O, U ²³⁴ O, U ²³³ O, and U ²³² O | | have similar alpha particle energies, therefore the energy and yield of the neutrons from the uranium oxide alpha, n reactions are similar. | | |
| Th ²³² O | 1.2 | 54 | 2E3 | 0.02 |
| | 1.2 | 54 | 2E3 | 0.02 |

Energy & Yield of neutrons from the alpha, n reaction

neutron
mrem/hr per Ci

| | η energy MeV | n/s/GBq | n/s/Ci | mrem/hr per Ci @ 30 cm |
|----------------------|----------------------|---------|--------|---------------------------|
| Ac ²²⁷ Be | av 5 | 7.02E5 | 2.6E7 | 289 |
| Ra ²²⁶ Be | av 4.5 | 5.02E5 | 1.9E7 | 211 |
| Ra ²²⁶ B | 3.0 | 8.0E4 | 3.0E5 | 3.3 |
| Po ²¹⁰ Be | 4.2 | 7.1E4 | 2.6E6 | 28.9 |
| Po ²¹⁰ Li | 0.48 | 1.2E3 | 4.4E4 | 0.49 |
| Po ²¹⁰ B | 2.5 | 1.0E3 | 3.7E5 | 4.1 |
| Po ²¹⁰ F | 0.42 | 3E3 | 1.1E5 | 1.2 |

Ra-226 and Ac-227 include progeny effects

Energy & Yield for 5.2 MeV alpha particles for various elements

| α , η sources | η energy (MeV) | n/s/GBq | n/s/Ci |
|---------------------------|---------------------|---------|--------|
| Li | 0.3 | 1.13E3 | 4.2E4 |
| Be | 4.2 | 6.5E4 | 2.4E6 |
| B | 2.9 | 1.75E4 | 6.5E5 |
| C | 4.4 | 7.8E1 | 2.9E3 |
| O | 1.9 | 5.9E1 | 2.2E3 |
| F | 1.2 | 5.9E3 | 2.2E5 |
| Na | ? | 1.1E3 | 4.1E4 |
| Mg | 2.7 | 8.9E2 | 3.3E4 |
| Al | 1.0 | 4.1E2 | 1.5E4 |
| Si | 1.2 | 7.6E1 | 2.8E3 |
| Cl | ? | 7E1 | 2.6E3 |

Isotopic Mix of WG Pu

| | Pu-238 | Pu-239 | Pu-240 | Pu-241 | Pu-242 |
|---|--------|--------|--------|--------|---------|
| % Weight | 0.02 | 93.16 | 6.43 | 0.33 | 0.06 |
| % Activity | 0.82 | 13.87 | 3.49 | 81.82 | 0.0006 |
| Curies for a 1 kilo-gram mixture of WG Pu | | | | | |
| | 3.42 | 57.9 | 14.6 | 339.9 | 2.36E-3 |
| exposure rates in rem/hr at 30 cm | | | | | |
| γ | 5.5E-4 | 7.5E-3 | 0.017 | --- | 1.2E-5 |
| η | --- | --- | --- | --- | 2.4E-5 |
| Total $\gamma + \eta$ | 0.025 | | | | |

Isotopic Mix of Heat Source (RTG) Pu238

| | Pu-238 | Pu-239 | Pu-240 | Pu-241 | Pu-242 |
|--|--------|--------|--------|--------|---------|
| % Weight | 90.0 | 9.10 | 0.60 | 0.30 | <0.01 |
| % Activity | 97.99 | 0.036 | 0.009 | 1.972 | 3.6E-6 |
| Curies for a 1 kilo-gram mixture of RTG Pu-238 | | | | | |
| | 1.54E4 | 5.65 | 1.36 | 309 | 6.48E-3 |
| exposure rates in rem/hr at 30 cm | | | | | |
| γ | 2.46 | 7.3E-4 | 1.6E-3 | --- | 3.2E-5 |
| η | --- | --- | --- | --- | 6.4E-5 |
| Total $\gamma + \eta$ | 2.46 | | | | |

Isotopic Mix of Reactor Grade Pu

| | Pu-238 | Pu-239 | Pu-240 | Pu-241 | Pu-242 |
|--|--------|--------|--------|--------|--------|
| % Weight | 1.50 | 58.1 | 24.1 | 11.4 | 4.90 |
| % Activity | 2.12 | 0.30 | 0.45 | 97.13 | 1.6E-3 |
| Curies for a 1 kilo-gram mixture of reactor grade Pu | | | | | |
| | 256.5 | 36.1 | 54.7 | 1.17E4 | 0.19 |
| exposure rates in rem/hr at 30 cm | | | | | |
| γ | 0.041 | 4.7E-3 | 0.063 | --- | 9.5E-4 |
| η | --- | --- | --- | --- | 1.9E-3 |
| Total $\gamma + \eta$ | 0.109 | | | | |

WG Pu 15 years after fabrication

| | Pu-238 | U-234 | Pu-239 | Pu-240 | Pu-241 | Pu-242 | Am-241 |
|--|--------|--------|--------|--------|--------|--------|--------|
| % Wt | 0.018 | 0.002 | 93.16 | 6.43 | 0.16 | 0.06 | 0.17 |
| % Act | 1.22 | 2.8E-4 | 23.43 | 5.86 | 67.24 | 6.0E-4 | 2.25 |
| Curies for a 1 kilo-gram mixture of 15 years-old WG Pu | | | | | | | |
| | 3.08 | 1.2E-4 | 57.85 | 14.6 | 164.8 | 2.4E-3 | 5.83 |
| exposure rates in rem/hr at 30 cm | | | | | | | |
| γ | 4.9E-4 | 3.6E-8 | 7.5E-3 | 0.017 | --- | 1.2E-5 | 0.991 |
| η | --- | --- | --- | --- | --- | 2.4E-5 | --- |
| Total $\gamma + \eta$ | 1.17 | | | | | | |

Heat Source (RTG) Pu238 15 years after fabrication

| | Pu-238 | U-234 | Pu-239 | Pu-240 | Pu-241 | Pu-242 | Am-241 |
|---|--------|--------|--------|--------|--------|--------|--------|
| % Wt | 79.94 | 10.06 | 9.10 | 0.60 | 0.14 | <0.01 | 0.16 |
| % Act | 99.00 | 1.2E-3 | 3.7E-5 | 9.1E-5 | 0.99 | 3.7E-8 | 3.7E-4 |
| Curies for a 1 kilo-gram mixture of 15 years-old RTG Pu-238 | | | | | | | |
| | 1.37E4 | 0.626 | 5.65 | 1.36 | 144.2 | 6.5E-3 | 5.49 |
| exposure rates in rem/hr at 30 cm | | | | | | | |
| γ | 2.19 | 1.9E-4 | 7.3E-4 | 1.6E-3 | --- | 3.3E-5 | 0.933 |
| η | --- | --- | --- | --- | --- | 6.6E-5 | --- |
| Total $\gamma + \eta$ | 3.13 | | | | | | |

Reactor Grade Pu 15 years after fabrication

| | Pu-238 | U-234 | Pu-239 | Pu-240 | Pu-241 | Pu-242 | Am-241 |
|--|--------|--------|--------|--------|--------|--------|--------|
| % Wt | 1.33 | 0.17 | 58.1 | 24.1 | 5.54 | 4.90 | 5.86 |
| % Act | 3.66 | 4.6E-5 | 0.58 | 0.88 | 91.83 | 3.1E-5 | 3.05 |
| Curies for 1 kilo-gram mixture of 15 year-old reactor grade Pu | | | | | | | |
| | 227.4 | 0.01 | 36.1 | 54.7 | 5.71E3 | 0.19 | 201 |
| exposure rates in rem/hr at 30 cm | | | | | | | |
| γ | 0.036 | 3E-6 | 4.7E-3 | 0.063 | --- | 9.5E-3 | 34.2 |
| η | --- | --- | --- | --- | --- | 1.9E-2 | --- |
| Total $\gamma + \eta$ | 34.3 | | | | | | |

**Neutron exposure rate
from the oxide form of radionuclides**

| mrem/hr per Ci at 30 cm | Pu-238 | U-234 | Pu-239 | Pu-240 | Pu-242 | Am-241 |
|----------------------------|--------|-------|--------|--------|--------|--------|
| | 2.5 | 2E-2 | 2.6E-5 | 3.6E-4 | 8.7E-8 | 0.1 |

**Neutron and gamma exposure rates from Spontaneous
Fission for Pu and U Power Source Radionuclides**

| | | | | | Spontaneous Fission | |
|---------|-----------|---------|----------------------|-----------|------------------------------|-----|
| | | | | | γ mrem /hr per Ci @ 30 cm | η |
| | Primary | | γ mrem /hr per Ci | S.F. | | |
| | Half-life | Ci / g | @ 30 cm | Half-life | γ | η |
| Pu-238 | 87.7y | 17.1 | 0.16 | 4.9E10y | --- | --- |
| U-234 | 2.45E5y | 6.22E-3 | 0.3 | 2E16y | --- | --- |
| Pu-239 | 2.41E4y | 6.21E-2 | 0.13 | 5.5E15y | --- | --- |
| Pu-240 | 6.56E3y | 0.227 | 0.16 | 1.39E11y | 1 | --- |
| Pu-241 | 14.4y | 103 | --- | --- | --- | --- |
| Am-241 | 432.7y | 3.43 | 170 | 2E14y | --- | --- |
| Pu-242 | 3.75E5y | 3.94E-3 | --- | 7E10y | 5 | 10 |
| U-238 | 4.47E9y | 3.36E-7 | 0.4 | 7E15y | 0.6 | 1.2 |
| Th-234 | 24.1d | 2.32E4 | 35.6 | --- | --- | --- |
| Pa-234m | 1.17m | 6.86E8 | 50 | --- | --- | --- |
| U-235 | 7.04E8y | 2.16E-6 | 755 | 1.9E17y | --- | --- |
| Th-231 | 25.22h | 5.32E5 | 48 | --- | --- | --- |
| U-234 | 2.46E5y | 6.22E-3 | 0.3 | 2E16 y | --- | --- |

Isotopic Mix of Natural U

| | U-238 | Th-234 | Pa-234m | U-235 | Th-231 | U-234 |
|---|--------|--------|---------|--------|--------|--------|
| % Wt | 99.27 | --- | --- | 0.72 | --- | 0.0057 |
| % Act | 24.39 | 24.39 | 24.39 | 1.16 | 1.16 | 24.51 |
| Curies for a 1 kilo-gram mixture of natural uranium | | | | | | |
| | 3.3E-4 | 3.3E-4 | 3.3E-4 | 1.6E-5 | 1.6E-5 | 3.5E-4 |
| gamma exposure rates in $\mu\text{rem}/\text{hr}$ at 30 cm | | | | | | |
| | 0.13 | 11 | 17 | 12 | 0.77 | 0.11 |
| Total gamma exposure rate 40 $\mu\text{rem}/\text{hr}$ at 30 cm | | | | | | |

Isotopic Mix of Commercial U

| | U-238 | Th-234 | Pa-234m | U-235 | Th-231 | U-234 |
|---|--------|--------|---------|--------|--------|--------|
| % Wt | 97.01 | --- | --- | 2.96 | --- | 0.03 |
| % Act | 11.23 | 11.23 | 11.23 | 2.27 | 2.27 | 61.76 |
| Curies for a 1 kilo-gram mixture of commercial uranium | | | | | | |
| | 3.3E-4 | 3.3E-4 | 3.3E-4 | 6.4E-5 | 6.4E-5 | 1.9E-3 |
| gamma exposure rates in $\mu\text{rem}/\text{hr}$ at 30 cm | | | | | | |
| | 0.13 | 11 | 17 | 48 | 3.1 | 0.57 |
| Total gamma exposure rate 79 $\mu\text{rem}/\text{hr}$ at 30 cm | | | | | | |

Isotopic Mix of 10% Enriched U

| | U-238 | Th-234 | Pa-234m | U-235 | Th-231 | U-234 |
|--|--------|--------|---------|--------|--------|--------|
| % Wt | 89.87 | --- | --- | 10.0 | --- | 0.13 |
| % Act | 3.25 | 3.25 | 3.25 | 2.32 | 2.32 | 85.59 |
| Curies for a 1 kilo-gram mixture of 10% enriched uranium | | | | | | |
| | 3.0E-4 | 3.0E-4 | 3.0E-4 | 2.2E-4 | 2.2E-4 | 8.1E-3 |
| gamma exposure rates in $\mu\text{rem}/\text{hr}$ at 30 cm | | | | | | |
| | 0.12 | 11 | 15 | 170 | 11 | 2.4 |
| Total gamma exposure rate 210 $\mu\text{rem}/\text{hr}$ at 30 cm | | | | | | |

Isotopic Mix of 20% Enriched U

| | U-238 | Th-234 | Pa-234m | U-235 | Th-231 | U-234 |
|--|--------|--------|---------|--------|--------|--------|
| % Wt | 79.68 | --- | --- | 20.0 | --- | 0.32 |
| % Act | 1.25 | 1.25 | 1.25 | 2.00 | 2.00 | 92.25 |
| Curies for a 1 kilo-gram mixture of 20% enriched uranium | | | | | | |
| | 2.7E-4 | 2.7E-4 | 2.7E-4 | 4.3E-4 | 4.3E-4 | 2.0E-2 |
| gamma exposure rates in μ rem/hr at 30 cm | | | | | | |
| | 0.11 | 9.6 | 14 | 320 | 21 | 6.0 |
| Total gamma exposure rate 370 μ rem/hr at 30 cm | | | | | | |

Isotopic Mix of Depleted U

| | U-238 | Th-234 | Pa-234m | U-235 | Th-231 | U-234 |
|--|--------|--------|---------|--------|--------|--------|
| % Wt | 99.75 | --- | --- | 0.25 | --- | 0.0005 |
| % Act | 32.01 | 32.01 | 32.01 | 0.53 | 0.53 | 2.90 |
| Curies for a 1 kilo-gram mixture of depleted uranium | | | | | | |
| | 3.4E-4 | 3.4E-4 | 3.4E-4 | 5.4E-6 | 5.4E-6 | 3.1E-5 |
| gamma exposure rates in μ rem/hr at 30 cm | | | | | | |
| | 0.14 | 12 | 17 | 4.1 | 0.26 | 9.3E-3 |
| Total gamma exposure rate 33 μ rem/hr at 30 cm | | | | | | |

Isotopic Mix of HEU

| | U-238 | Th-234 | Pa-234m | U-235 | Th-231 | U-234 |
|--|--------|--------|---------|--------|--------|--------|
| % Wt | 6.7 | --- | --- | 93.2 | --- | 0.01 |
| % Act | 0.5 | 0.5 | 0.5 | 42.6 | 42.6 | 13.3 |
| Curies for a 1 kilo-gram mixture of HEU | | | | | | |
| | 2.3E-5 | 2.3E-5 | 2.3E-5 | 2.0E-3 | 2.0E-3 | 6.2E-4 |
| gamma exposure rates in μ rem/hr at 30 cm | | | | | | |
| | 9.2E-3 | 0.82 | 1.2 | 1500 | 96 | 0.19 |
| Total gamma exposure rate 1.6 mrem/hr at 30 cm | | | | | | |

MISCELLANEOUS RULES OF THUMB

1. One watt of power in a reactor requires 3.1E10 fissions per second. In a reactor operating for more than 4 days, the total fission products are about 3 Ci / watt at 1.5 min after shutdown. At 2 years after shutdown, the fission products are approximately 75 Ci / MW-day.
2. The quantity of a short-lived fission product in a reactor which has been operated about four times as long as the half-life is given by; $Ci \sim (FY)(PL)$, where FY is the fission yield (%/100) and PL is the power level in watts.
3. Correction factor for unsealed ion chambers to STP ($0^{\circ}C$ and 760 mm of Hg) is $f = (t + 273)/(273) \times (760 / P)$ where t is the ambient temperature in degrees C and P is the ambient barometric pressure in mm of Hg.
4. The activity of an isotope (without radioactive daughter) is reduced to less than 1% after seven half-lives.

5. NATURALLY OCCURRING RADIONUCLIDES

| Primordial | Cosmogonic |
|-------------------|-------------------|
| K-40 | Tritium |
| Rb-87 | Be-7 |
| Natural U and Th | C-14 |

6. Unified Time, Distance, and Shielding formula for reduction of external dose.

$$\text{Rem} = \text{Initial Rem/hr} \times T \text{ in hours} \times (D_2)^2/(D_1)^2 \times 0.5^n$$

Where: Rem is the dose after applying reduction methods
T is the exposure time in hours
 D_1 is the initial distance to the source
 D_2 is the new distance to the source
 0.5^n is the Shielding for 'n' half-value layers

UNITS AND TERMINOLOGY

| | “Special Units” | SI Units |
|-----------------|---|-------------------|
| Exposure | Roentgen | Coulombs / kg |
| Dose | rad (0.01 Gy) | Gray (100 rad) |
| Dose Equiv | rem (0.01 Sv) | Sievert (100 rem) |
| Activity | Curie (2.22 E12 dpm) | Becquerel (1dps) |
| 1 Roentgen | = 2.58 E-4 coulomb / kg in air | |
| | = 1 esu / cm ³ in air | |
| | = 87.7 ergs / gm in air | |
| | = 98 ergs / gm in soft tissue | |
| 1 rad | = 100 ergs / gm in any absorber | |
| 1 Gray | = 10,000 ergs / gm in any absorber | |
| 1 rem | = 1 rad x QF = 0.01 Sv | |
| H | = DQN (from ICRP 26) | |
| H (Dose Equiv.) | = D (absorbed dose) x Q (quality factor) x N (any other modifying factors) | |

DEFINITIONS

| | |
|-----------------------------------|--|
| Acute | any dose in a short period of time |
| Chronic | any dose in a long period of time |
| Somatic | effects in the exposed individual |
| Genetic | effects in the offspring of the exposed individual |
| Teratogenic | effects in the exposed unborn embryo/fetus |
| Stochastic | effects for which a probability exists and increases with increasing dose |
| Non-Stochastic (deterministic) | effects for which a threshold exists - effects do not occur below the threshold (examples; cataracts, erythema, epilation, acute radiation syndrome) |

PUBLIC RADIATION DOSES

| | |
|---|-------------------------------|
| Average per capita US Dose | 200 mrem (2 mSv) / yr |
| Living in Los Alamos (7000' elev) | 327 mrem (3.27 mSv)/yr |
| Flying from NY to LA | 2.5 mrem (25 μ Sv) / trip |
| Chest x-ray | 10 mrem (0.1mSv)/exam |
| Full mouth dental x-ray | 9 mrem (90 μ Sv) / exam |
| The external dose rate for cosmic rays doubles for each mile increase in elevation. | |

BACKGROUND RADIATION

| | | |
|---|---|-----------------------------------|
| Cosmic | = | 28 mrem (0.28 mSv) / yr |
| Rocks | = | 28 mrem (0.28 mSv) / yr |
| Internal | = | 36 mrem (0.36 mSv) / yr |
| Medical x-rays | = | 20 to 30 mrem (0.2 to 0.3 mSv)/yr |
| Nuclear medicine | = | 2 mrem / yr |
| TOTAL US Ave | ~ | 120 mrem / yr |
| US Ave H ϵ from radon | = | 200 mrem / yr |
| Ave H ϵ from medical x-ray procedures: | | |
| Skull 20 mrem (0.2 mSv) | | |
| Upper GI 245 mrem (2.45 mSv) | | |
| Hip 65 mrem (0.65 mSv) | | |
| Chest 6 mrem (60 μ Sv), | | |
| Kidney 55 mrem (0.55 mSv) | | |
| Dental 55 mrem (0.55 mSv) | | |

| Occupational Doses | mrem/yr | mSv/yr |
|-------------------------------|----------------|---------------|
| airline flight crew | 1,000 | 10 |
| nuclear power plant | 700 | 7 |
| Grand Central Station workers | 120 | 1.2 |
| medical personnel | 70 | 0.7 |
| DOE employees | 44 | 0.44 |

RADON FACTS

1 working level = 3 DAC Rn-222 (including progeny)
= 1.3E5 MeV / liter of air α energy
= 100 pCi / liter (1E-7 uCi / mL)
= 20.8 μ Joules / M3

1 working level-month = 1 pCi / L in air thru evaporation

EPA ACTION LEVELS FOR RADON GAS IN HOMES

| Concentration (pCi / L) | Sampling Frequency |
|--|-----------------------------------|
| 0 – 4 | initial and no follow up |
| EPA Recommends Mitigation at > 4 pCi / L | |
| 4 -20 | one year and follow up |
| 20 -200 | 3 months and follow up |
| > 200 | Implement radon reduction methods |

4 pCi / L in living area = 1.03 working level-month = 1 rem

PROPOSED EPA ACTION LEVELS FOR RADON IN DRINKING WATER

Maximum Contaminant Level (MCL) is 300 pCi / L of radon in water of community water systems (CWS).

Alternative Maximum Contaminant Level (AMCL) is 4,000 pCi / L of radon in water of community water systems.

To comply with the AMCL limit the state or the CWS (Community Water System) must implement a Multi-Media Mitigation plan to address the radon in the air of residences. The proposed rule would not apply to CWSs that use solely surface water.

The proposed rule requires monitoring for radon in drinking water. The monitoring frequency varies from once per quarter to once in 9 years based on radon concentrations.

COMPARATIVE RISKS OF RADIATION EXPOSURE

Estimated Days of Life Lost

| | |
|------------------------------------|-------|
| Smoking 1 pack of cigarettes / day | 2,370 |
| 20% overweight | 985 |
| Average US alcohol consumption | 130 |
| Home accidents | 95 |

OCCUPATIONAL RISKS

| Occupation | Estimated Days of Life Lost |
|---|------------------------------------|
| demolition | 1,500 |
| mining | 1,100 |
| firefighting | 800 |
| railroad | 500 |
| farming | 300 |
| construction | 200 |
| transportation & public utilities | 160 |
| average of all occupations | 60 |
| government | 55 |
| radiation dose of 1 rem (10 mSv) per year | 50 |
| service | 45 |
| trade | 30 |
| single radiation dose of 1 rem (10 mSv) | 1.5 |

Relative Risk - U.S. National Vital Statistics Report for 2010

| | Number of Deaths | Percent |
|---|------------------|---------|
| All causes | 2,468,435 | 100.0 |
| Heart disease | 597,689 | 24.2 |
| Malignant neoplasms | 574,743 | 23.3 |
| Chronic lower respiratory diseases | 138,080 | 5.6 |
| Cerebrovascular diseases | 129,476 | 5.2 |
| Alzheimer's disease | 83,494 | 3.4 |
| Diabetes mellitus | 69,071 | 2.8 |
| Nephritis, nephrotic syndrome & nephrosis | 50,476 | 2.0 |
| Influenza and pneumonia | 50,097 | 2.0 |
| Suicide | 38,364 | 1.6 |
| Septicemia | 34,812 | 1.4 |
| Motor vehicle accidents | 33,783 | 1.4 |
| Chronic liver disease and cirrhosis | 31,903 | 1.3 |
| Essential hypertension and hypertensive renal disease | 26,634 | 1.1 |
| Parkinson's disease | 22,032 | 0.9 |
| Pneumonitis due to solids and liquids | 17,011 | 0.7 |
| Falling | 11,323 | 0.46 |
| Firearm assault | 7,861 | 0.32 |
| Pedestrian accident | 3,943 | 0.16 |
| Drowning | 2,449 | 0.099 |
| Motorcycle accident | 2,420 | 0.098 |
| Fire or smoke | 2,217 | 0.0898 |
| Bicycle accident | 502 | 0.0203 |
| Air / space accident | 489 | 0.0198 |
| Accidental firearm discharge | 481 | 0.0195 |
| Accidental electrocution | 248 | 0.0100 |
| Alcohol poisoning | 246 | 0.00995 |
| Hot weather | 180 | 0.00728 |
| Hornet, wasp, or bee sting | 43 | 0.00176 |
| Remaining causes of death are <43 individuals per cause. | 538,278 | 21.8 |

WEBSITES OF INTEREST

www.cdc.gov
www.defenselink.mil
www.dot.gov
www.eh.doe.gov/nepa
www.epa.gov/radiation
www.fedworld.gov
www.lanl.gov
www.lib.lsu.edu/gov/alpha
www.nrc.gov
html www.ornl.gov
www.osha.gov
www.aarst.org
www.acgih.org
www.amug.us
www.ansi.org
www.icrp.org
www.sra.org
www.ncrp.com
www.nrrpt.org
www.nrsi.org
www.radres.org

www.cirms.tis.doe.gov
www.dnfsb.gov
www.edf.fr
www.energy.gov
www.fda.gov/cdrh
www.fema.gov
www.lbl.gov
www.llnl.gov
www.doe.gov
www.sandia.gov
www.srs.gov
www.hps.org
www.aiha.org
www.ans.org
www.cea.fr
www.iaea.org
www.irpa.net
www.nea.fr
www.nrsb.org
www.nuclearsafety.gc.ca
www.rsna.org